

عنوان آزمایش : Alpha Fetoprotein - CLIA
عنوان دستگاه : elecsys

سری ساخت : 405843

عنوان کنترل : TUMOR MAEKER - HIGH
شروع کنترل : 1399/08/27:


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
116.216	107.595	98.974	90.353	81.732	73.111	64.49	8.621	9.542

تاریخ	مقدار
23/10/1400	90.1
25/10/1400	80.8
26/10/1400	83.6
27/10/1400	83.7
28/10/1400	85.5
29/10/1400	91.4

تاریخ	مقدار
12/10/1400	78.4
13/10/1400	78.9
14/10/1400	78.1
15/10/1400	95
18/10/1400	95.5
19/10/1400	83.8
20/10/1400	85.5
21/10/1400	93.2
22/10/1400	82.5

تاریخ	مقدار
01/10/1400	105.2
02/10/1400	101.9
04/10/1400	96.96
05/10/1400	99.04
06/10/1400	100.7
07/10/1400	89.09
08/10/1400	79.02
11/10/1400	79.67
11/10/1400	87.2

Mean: 88.532	SD: 8.259	CV%: 9.329
--------------	-----------	------------

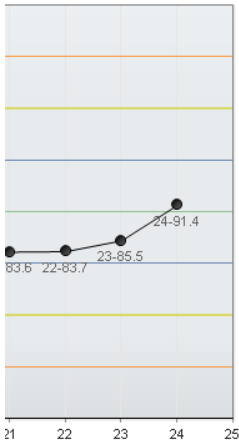

TUMOR MAEKER -HIGH

عنوان کنترل

CV% 9.542 SD 8.621 -3SD 64.49 -2SD 73.111 -1SD 81.732 Mean 90.353 1SD 98.974 2SD 107.595 3SD 116.216

اطلاعات

سری ساخت : 405843

آرشیو

شروع کنترل : 1399/08/27

مقدار

تاریخ

مقدار	تاریخ
101.9	1400/10/02
96.96	1400/10/04
99.04	1400/10/05
100.7	1400/10/06
89.09	1400/10/07
79.02	1400/10/08
79.67	1400/10/11
87.2	1400/10/11
78.4	1400/10/12
78.9	1400/10/13
78.1	1400/10/14
95	1400/10/15
95.5	1400/10/18
83.8	1400/10/19
85.5	1400/10/20
93.2	1400/10/21
82.5	1400/10/22
90.1	1400/10/23
80.8	1400/10/25
83.6	1400/10/26
83.7	1400/10/27
85.5	1400/10/28
91.4	1400/10/29


Mean: 88.532

SD: 8.259

CV%: 9.329

6σ

elecsys

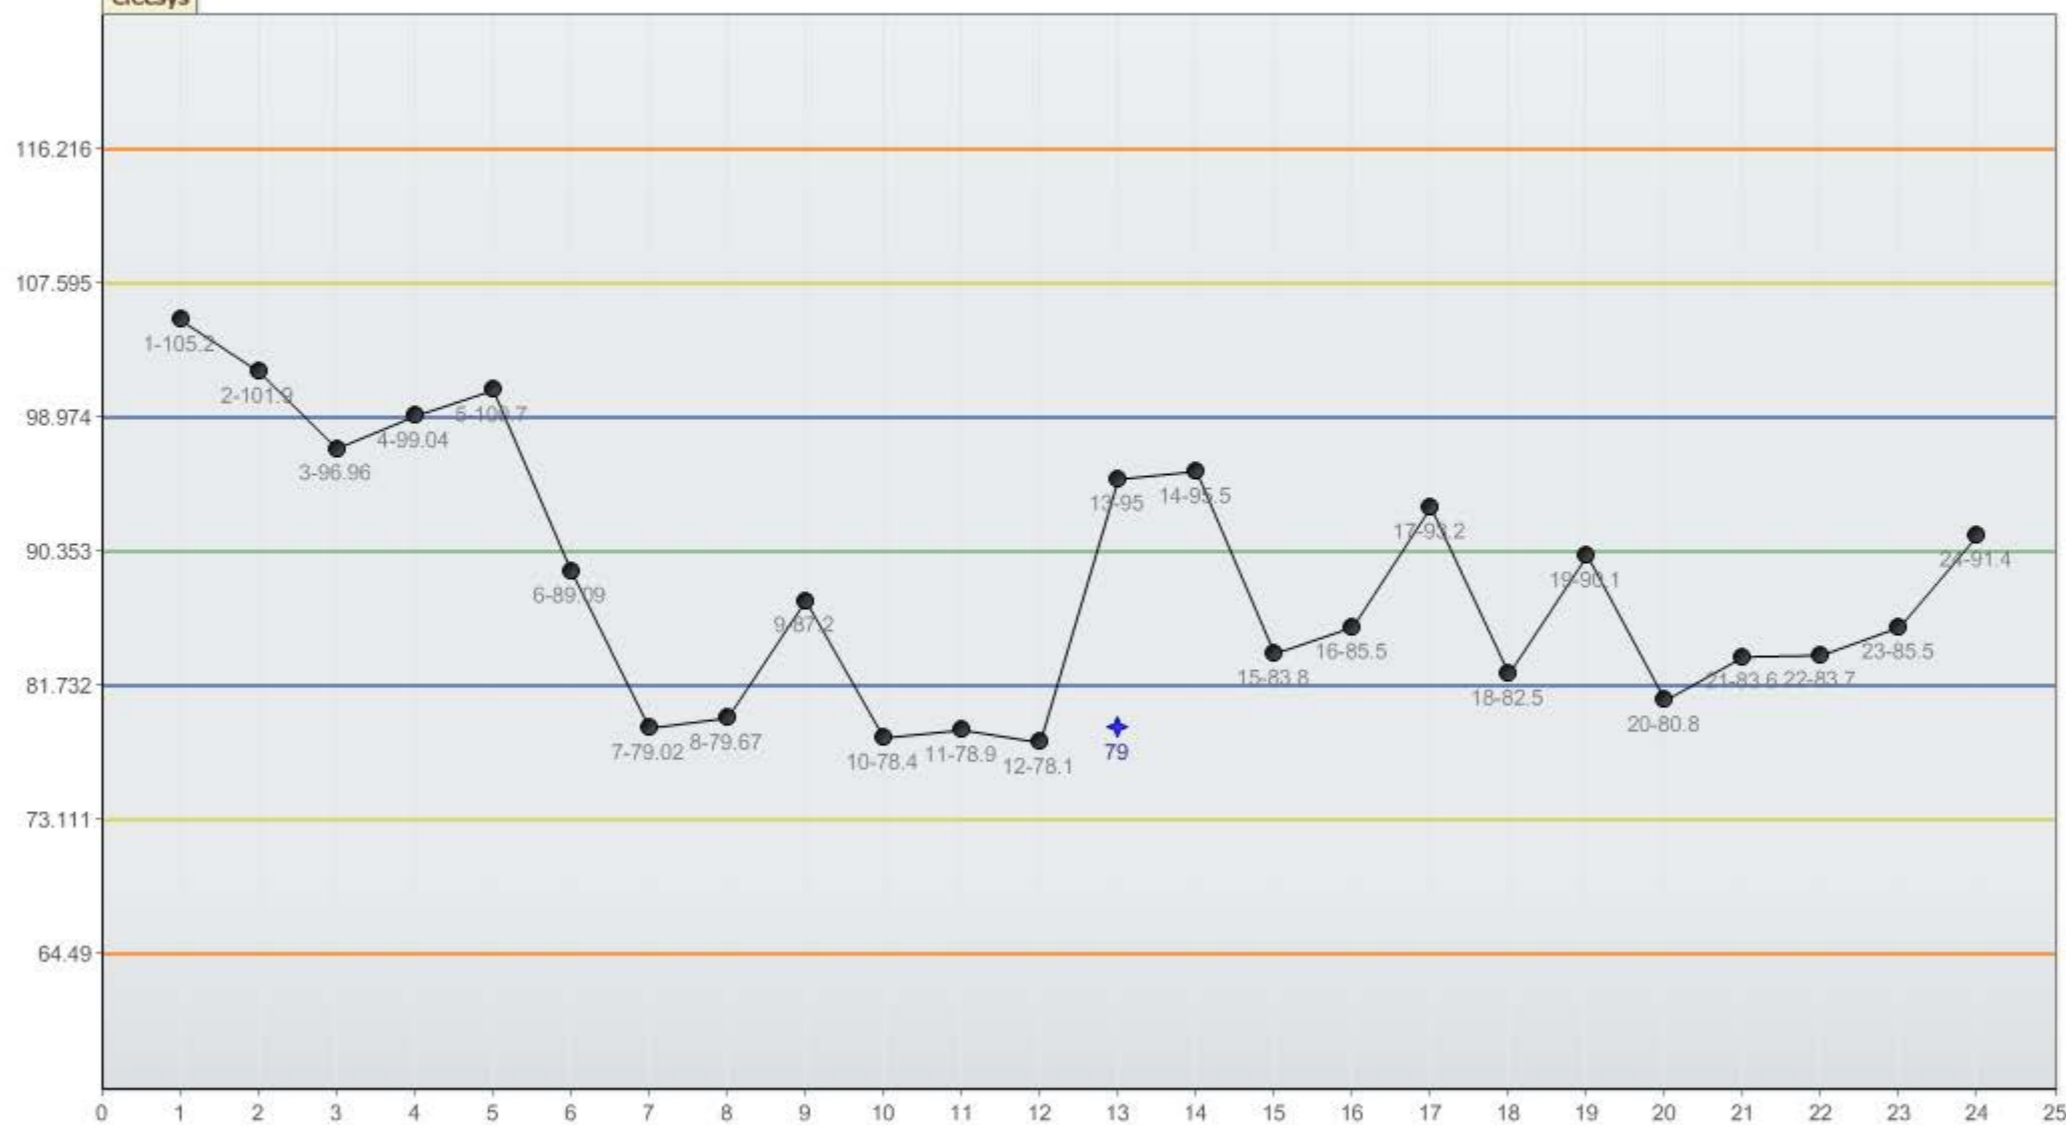

عنوان آزمایش : Alpha Fetoprotein -CLIA
عنوان دستگاه : Elecsys

سری ساخت : 405844

عنوان کنترل : TUMOR MAEKER -N
شروع کنترل :
1399/08/27:


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
10.375	9.675	8.975	8.275	7.575	6.875	6.175	0.7	8.46

تاریخ	مقدار
23/10/1400	8.1
25/10/1400	7.3
26/10/1400	7.79
27/10/1400	7.7
28/10/1400	7.9
29/10/1400	8.6

تاریخ	مقدار
11/10/1400	8.3
12/10/1400	8.8
13/10/1400	7.7
14/10/1400	7.7
15/10/1400	7.26
18/10/1400	8
19/10/1400	9.8
20/10/1400	8.4
21/10/1400	7.7

تاریخ	مقدار
01/10/1400	8.84
02/10/1400	8.97
04/10/1400	7.72
05/10/1400	8.4
06/10/1400	7.97
07/10/1400	8.63
08/10/1400	7.79
09/10/1400	7.99
11/10/1400	7.67

Mean: 8.126	SD: 0.59	CV%: 7.26
-------------	----------	-----------

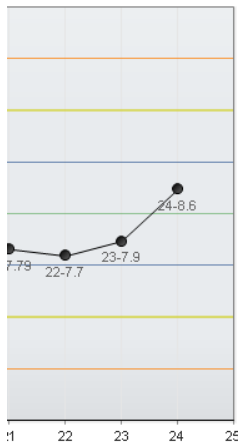



TUMOR MAEKER -N

عنوان کنترل

CV% 8.46 SD 0.7 -3SD 6.175 -2SD 6.875 -1SD 7.575 Mean 8.275 1SD 8.975 2SD 9.675 3SD 10.375

اطلاعات

سری ساخت : 405844

آرشیو

شروع کنترل : 1399/08/27

مقدار	تاریخ
8.84	1400/10/01
8.97	1400/10/02
7.72	1400/10/04
8.4	1400/10/05
7.97	1400/10/06
8.63	1400/10/07
7.79	1400/10/08
7.99	1400/10/09
7.67	1400/10/11
8.3	1400/10/11
8.8	1400/10/12
7.7	1400/10/13
7.7	1400/10/14
7.26	1400/10/15
8	1400/10/18
9.8	1400/10/19
8.4	1400/10/20
7.7	1400/10/21
8.1	1400/10/23
7.3	1400/10/25
7.79	1400/10/26
7.7	1400/10/27
7.9	1400/10/28
8.6	1400/10/29

Mean: 8.126 SD: 0.59 CV%: 7.26 6σ

Elecsys

