

CV% 7.544 SD 7.182 -3SD 73.651 -2SD 80.833 -1SD 88.015 Mean 95.197 1SD 102.379 2SD 109.561 3SD 116.743

چاپ

TUMOR MAEKER -HIGH

عنوان کنترل

اطلاعات

سری ساخت : 405843

آرشیو

شروع کنترل : 1399/08/27

مقدار تاریخ

مقدار	تاریخ
94.55	1400/09/01
91.69	1400/09/02
99.4	1400/09/03
94.9	1400/09/04
99.25	1400/09/06
90.2	1400/09/07
89.02	1400/09/08
78.32	1400/09/09
89.17	1400/09/10
82.44	1400/09/11
92.18	1400/09/13
98.77	1400/09/14
78.85	1400/09/15
81.32	1400/09/16
90.73	1400/09/17
88.52	1400/09/18
105.1	1400/09/20
101.7	1400/09/21
92.11	1400/09/22
89.14	1400/09/23
87.31	1400/09/24
93.59	1400/09/25
98.01	1400/09/27
102.9	1400/09/28
102.1	1400/09/29


Mean: 92.814

SD: 7.493

CV%: 8.073

6σ

elecsys

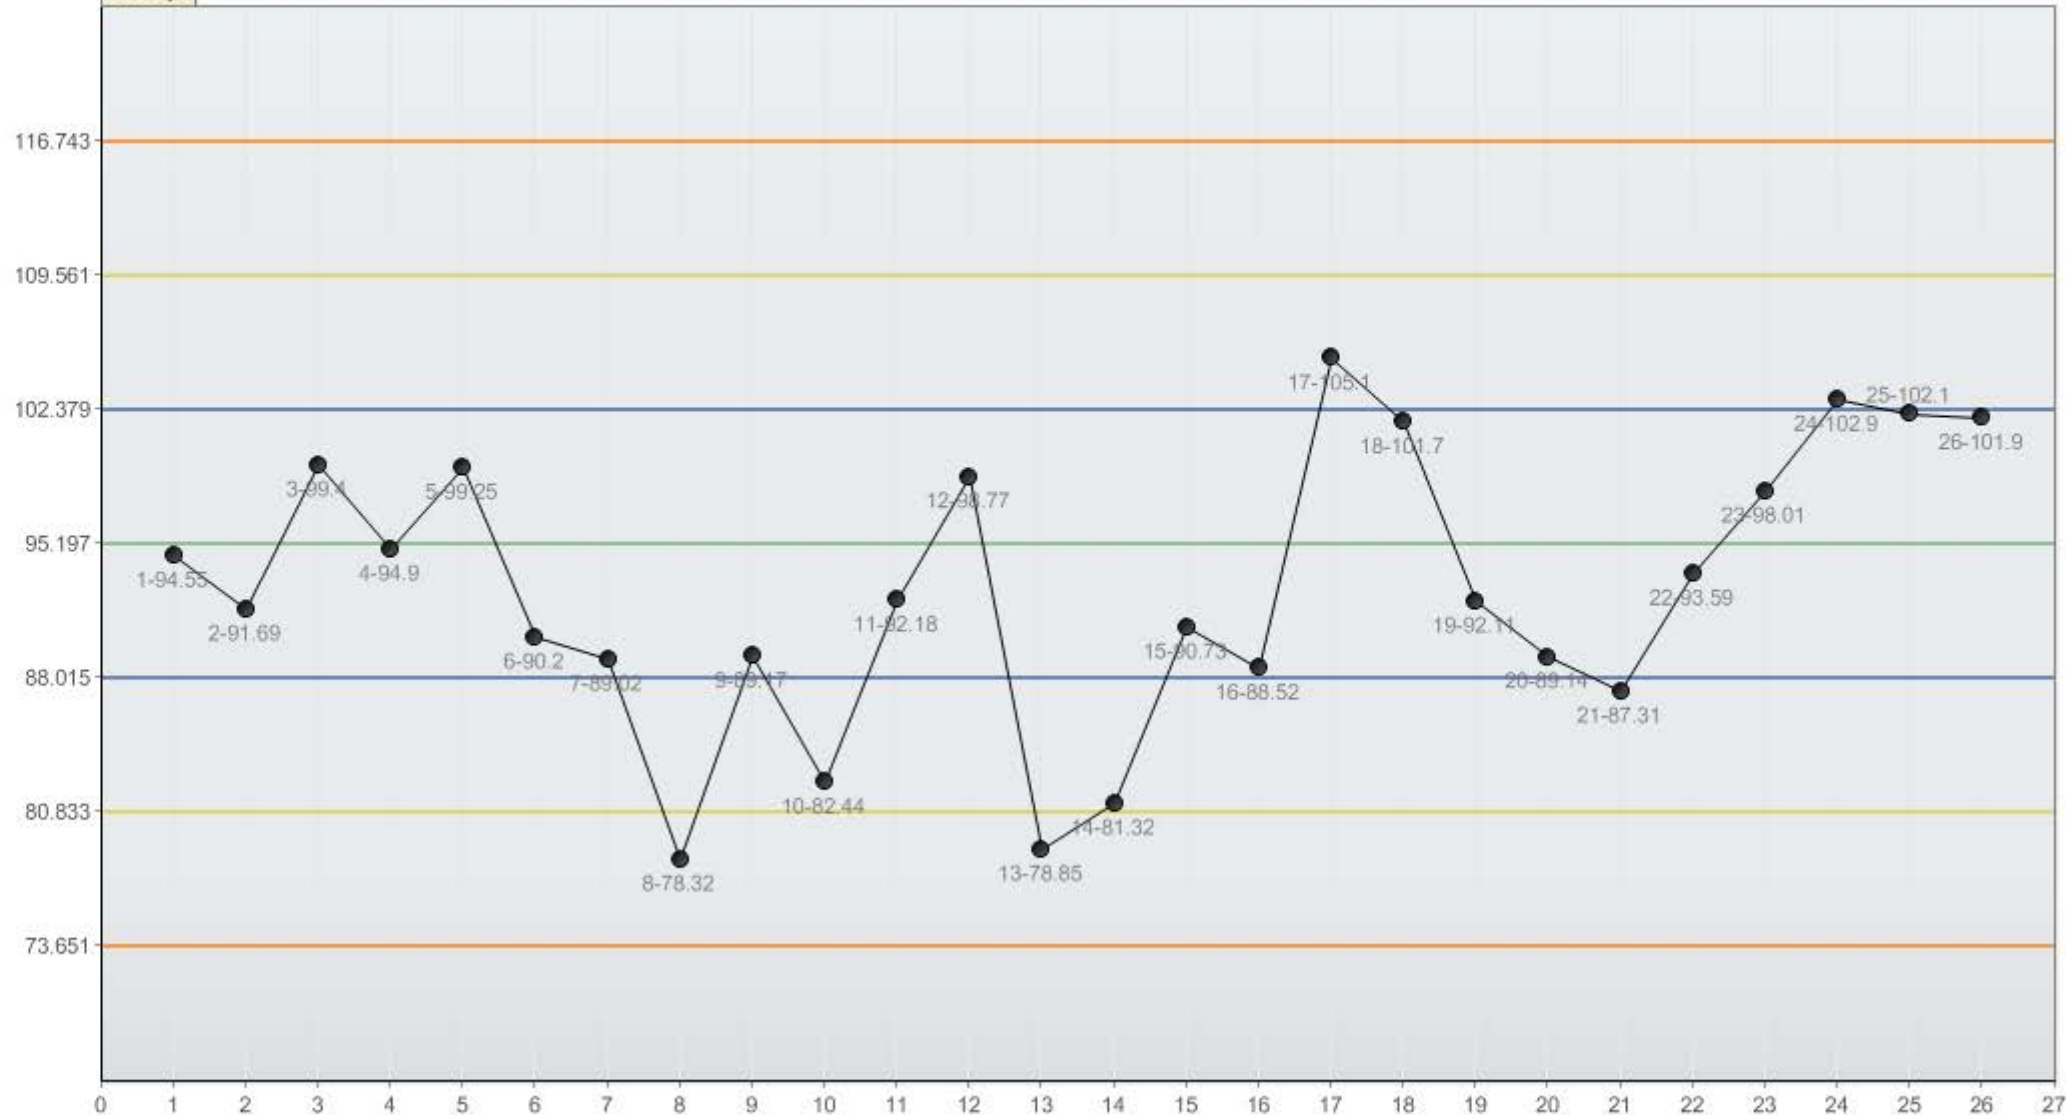

عنوان آزمایش : Alpha Fetoprotein -  
CLIA  
عنوان دستگاه : elecsys

سری ساخت : 405843

عنوان کنترل : TUMOR MAEKER -  
HIGH  
شروع کنترل :  
1399/08/27:

3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
116.743	109.561	102.379	95.197	88.015	80.833	73.651	7.182	7.544

تاریخ	مقدار
22/09/1400	92.11
23/09/1400	89.14
24/09/1400	87.31
25/09/1400	93.59
27/09/1400	98.01
28/09/1400	102.9
29/09/1400	102.1
30/09/1400	101.9

تاریخ	مقدار
11/09/1400	82.44
13/09/1400	92.18
14/09/1400	98.77
15/09/1400	78.85
16/09/1400	81.32
17/09/1400	90.73
18/09/1400	88.52
20/09/1400	105.1
21/09/1400	101.7

تاریخ	مقدار
01/09/1400	94.55
02/09/1400	91.69
03/09/1400	99.4
04/09/1400	94.9
06/09/1400	99.25
07/09/1400	90.2
08/09/1400	89.02
09/09/1400	78.32
10/09/1400	89.17

TUMOR MAEKER -N

عنوان کنترل

CV% 7.197 SD 0.608 -3SD 6.623 -2SD 7.231 -1SD 7.839 Mean 8.447 1SD 9.055 2SD 9.663 3SD 10.271

چاپ

اطلاعات

سری ساخت : 405844


آرشیو

شروع کنترل : 1399/08/27

مقدار	تاریخ
8.86	1400/09/01
8.25	1400/09/02
7.83	1400/09/03
7.5	1400/09/04
7.56	1400/09/06
8.24	1400/09/07
8.8	1400/09/08
8.13	1400/09/09
8.11	1400/09/10
9.07	1400/09/11
8.9	1400/09/13
8.7	1400/09/14
7.91	1400/09/15
8.74	1400/09/16
8.8	1400/09/17
7.14	1400/09/18
9.4	1400/09/20
8.82	1400/09/21
8.88	1400/09/22
8.69	1400/09/23
8.87	1400/09/24
9.78	1400/09/25
7.65	1400/09/27
9.03	1400/09/28
9.72	1400/09/29

Mean: 8.522 SD: 0.672 CV%: 7.887 6σ

Elecsys

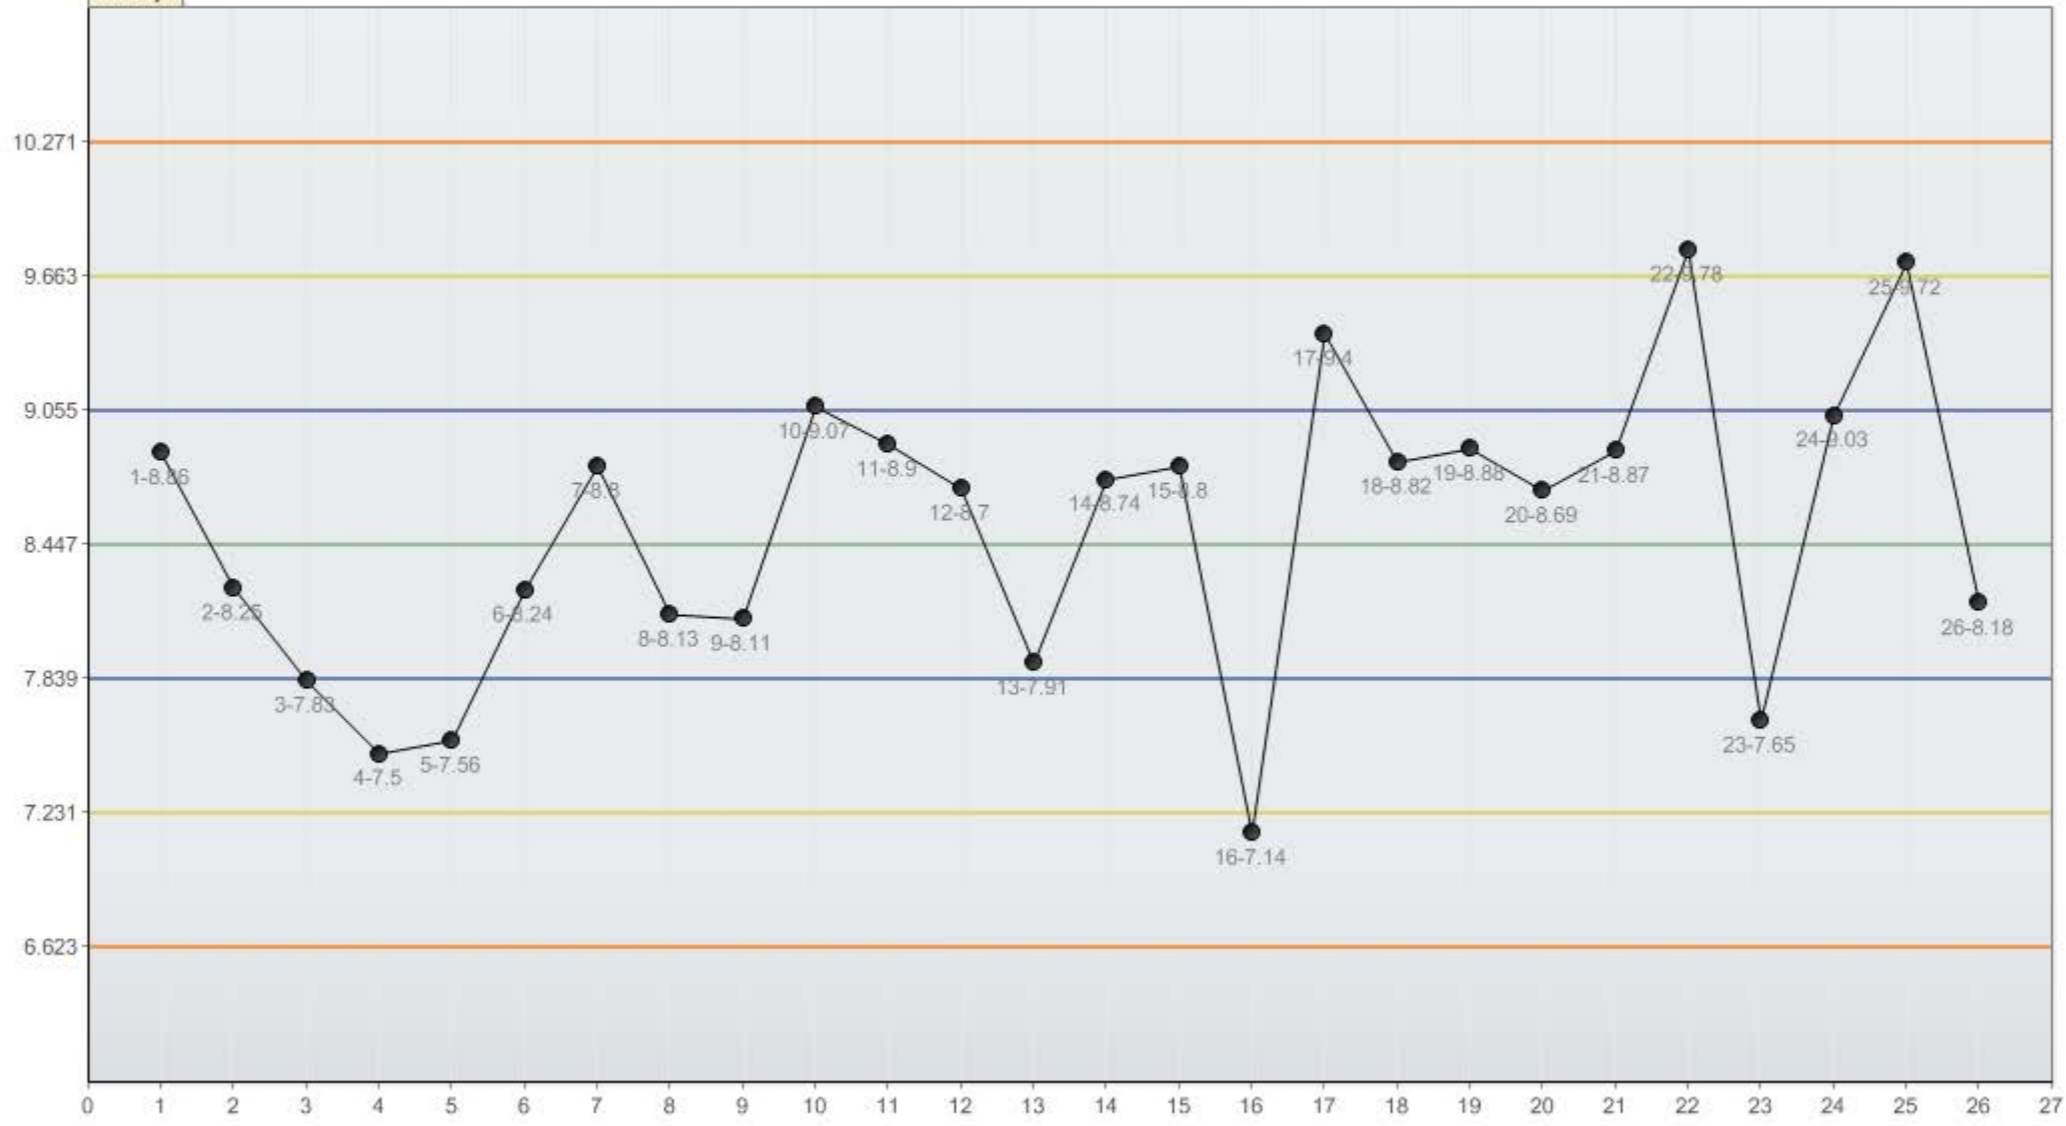

عنوان آزمایش : Alpha Fetoprotein -CLIA

عنوان دستگاه : Elecsys

سری ساخت : 405844

عنوان کنترل :

شروع کنترل

1399/08/27:

TUMOR MAEKER -N

3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
10.271	9.663	9.055	8.447	7.839	7.231	6.623	0.608	7.197

تاریخ	مقدار
22/09/1400	8.88
23/09/1400	8.69
24/09/1400	8.87
25/09/1400	9.78
27/09/1400	7.65
28/09/1400	9.03
29/09/1400	9.72
30/09/1400	8.18

تاریخ	مقدار
11/09/1400	9.07
13/09/1400	8.9
14/09/1400	8.7
15/09/1400	7.91
16/09/1400	8.74
17/09/1400	8.8
18/09/1400	7.14
20/09/1400	9.4
21/09/1400	8.82

تاریخ	مقدار
01/09/1400	8.86
02/09/1400	8.25
03/09/1400	7.83
04/09/1400	7.5
06/09/1400	7.56
07/09/1400	8.24
08/09/1400	8.8
09/09/1400	8.13
10/09/1400	8.11