

عنوان آزمایش : CA-125

عنوان دستگاه : abbot 34312201 : سری ساخت

عنوان کنترل :

abbot-I

شروع کنترل : 1400/09/18


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
16.601	15.324	14.047	12.77	11.493	10.216	8.939	1.277	4.3

تاریخ	مقدار
20/10/1400	11.4
21/10/1400	11.3
22/10/1400	12.5
23/10/1400	12.9
25/10/1400	12.5
26/10/1400	12.8
27/10/1400	11
28/10/1400	11.5
29/10/1400	13.9
30/10/1400	12.3
02/11/1400	12

تاریخ	مقدار
04/10/1400	12.8
05/10/1400	11.8
06/10/1400	11.9
07/10/1400	12
08/10/1400	11
09/10/1400	12.9
11/10/1400	11.6
12/10/1400	11.2
13/10/1400	11.6
14/10/1400	10.8
15/10/1400	10.7
18/10/1400	11
19/10/1400	13.1

تاریخ	مقدار
18/09/1400	11.1
20/09/1400	12
21/09/1400	11.6
22/09/1400	11.8
23/09/1400	12.2
24/09/1400	11.9
25/09/1400	12.2
27/09/1400	12.8
28/09/1400	11.5
29/09/1400	11.9
30/09/1400	12.1
01/10/1400	11.4
02/10/1400	11.6

Mean: 11.908	SD: 0.722	CV%: 6.063
--------------	-----------	------------

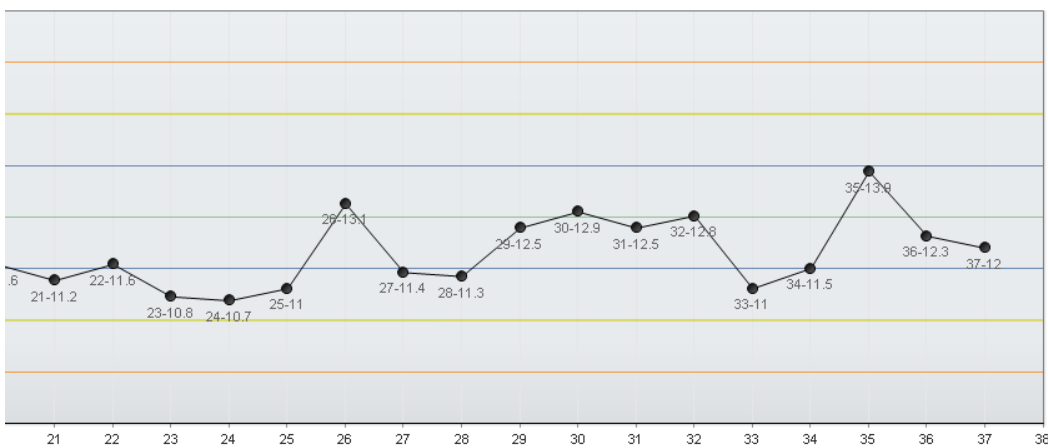

CV% 4.3 SD 1.277 -3SD 8.939 -2SD 10.216 -1SD 11.493 Mean 12.77 1SD 14.047 2SD 15.324 3SD 16.601

جواب


abbott-I عنوان کنترل

اطلاعات سری ساخت : 34312201

آرشیو شروع کنترل : 1400/09/18

مقدار	تاریخ
11.8	1400/10/05
11.9	1400/10/06
12	1400/10/07
11	1400/10/08
12.9	1400/10/09
11.6	1400/10/11
11.2	1400/10/12
11.6	1400/10/13
10.8	1400/10/14
10.7	1400/10/15
11	1400/10/18
13.1	1400/10/19
11.4	1400/10/20
11.3	1400/10/21
12.5	1400/10/22
12.9	1400/10/23
12.5	1400/10/25
12.8	1400/10/26
11	1400/10/27
11.5	1400/10/28
13.9	1400/10/29
12.3	1400/10/30
12	1400/11/02

Mean: 11.908 SD: 0.722 CV%: 6.063 6σ

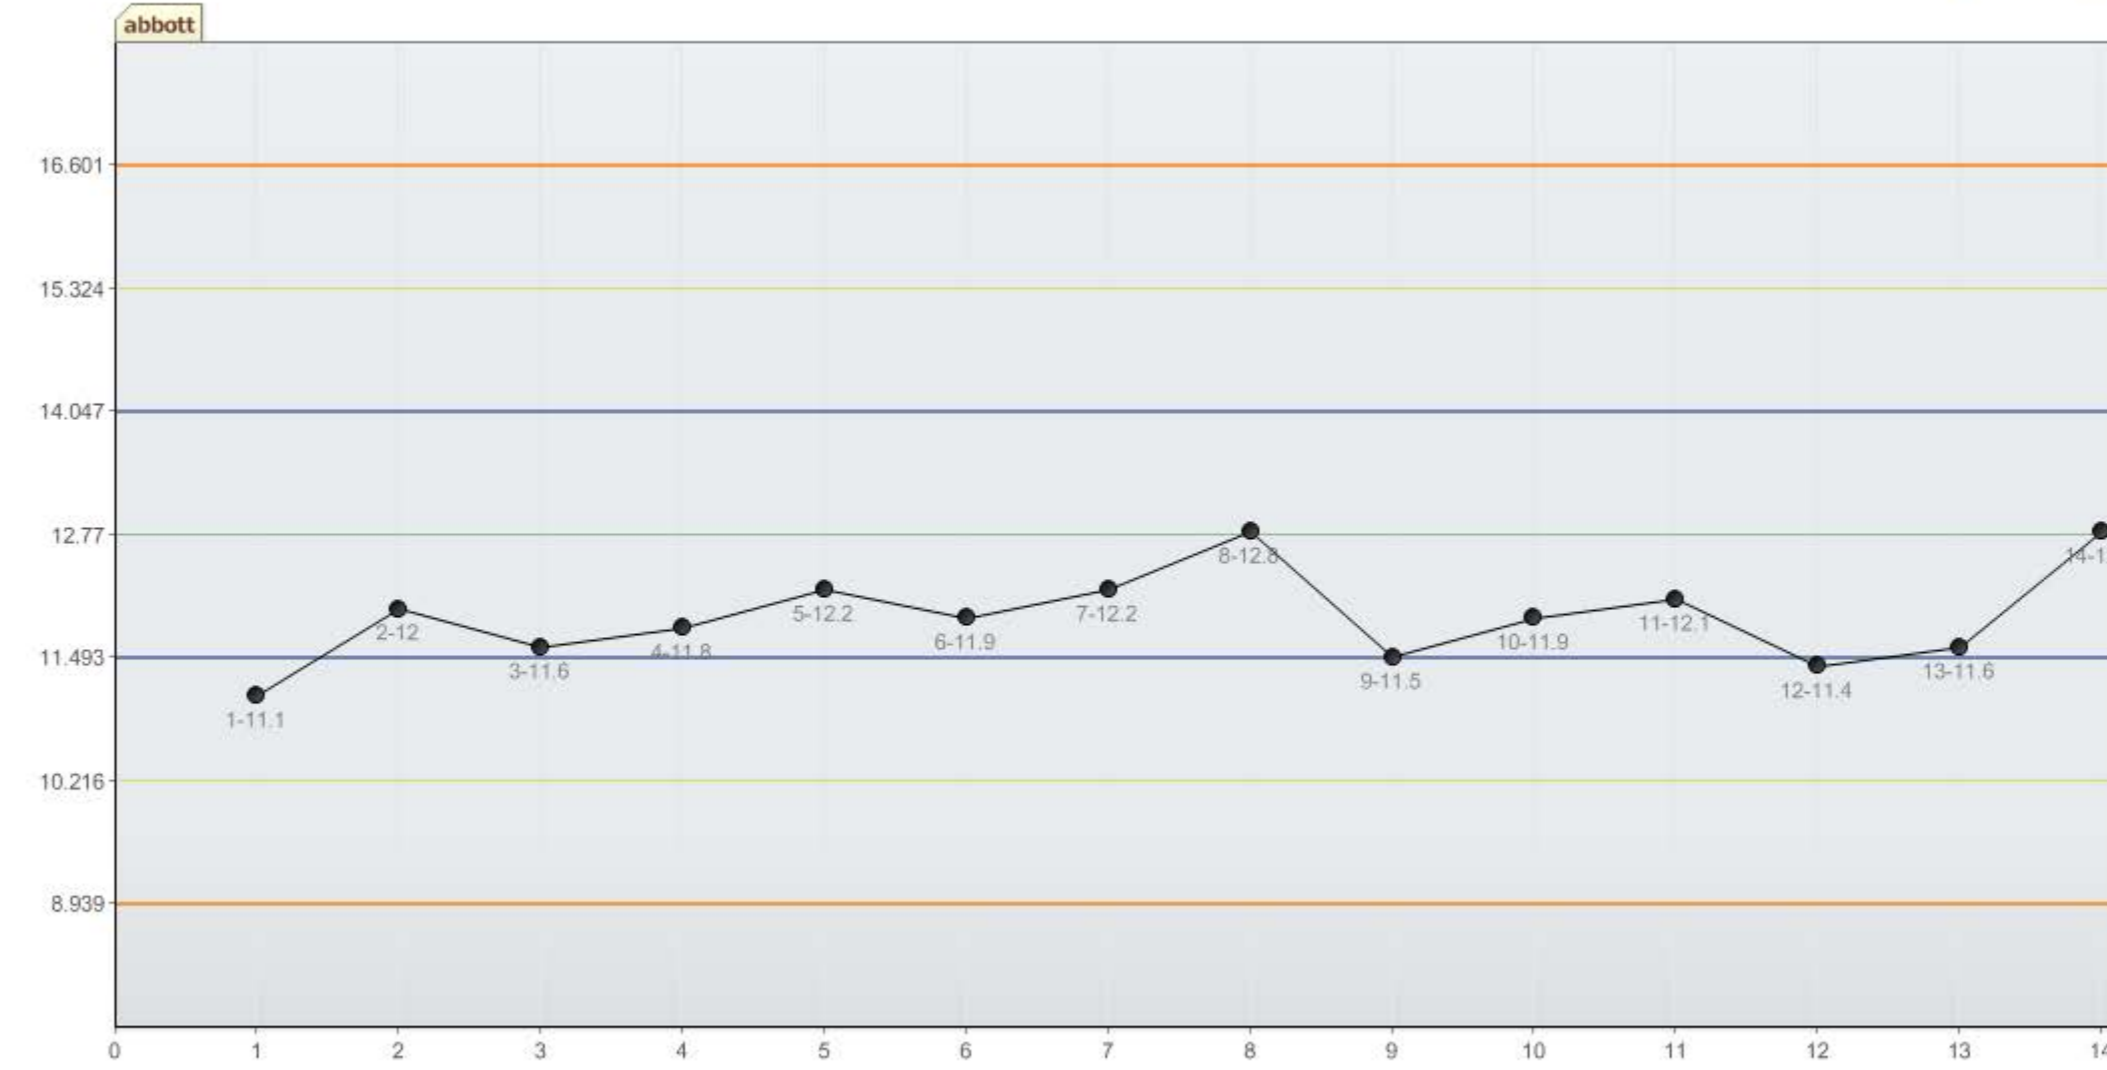

عنوان آزمایش : CA-125

عنوان دستگاه : abbot 34312203 : سری ساخت

عنوان کنترل :

abbott-III

شروع کنترل : 1400/09/18


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
106.001	100.134	94.267	88.4	82.533	76.666	70.799	5.867	4.3

تاریخ	مقدار
20/10/1400	79.2
21/10/1400	78.5
22/10/1400	87.4
23/10/1400	84
25/10/1400	86.9
26/10/1400	84.9
27/10/1400	79.4
28/10/1400	78
29/10/1400	91
30/10/1400	83.9
02/11/1400	83.5

تاریخ	مقدار
04/10/1400	83.4
05/10/1400	83.3
06/10/1400	80
07/10/1400	88.5
08/10/1400	83.9
09/10/1400	81.7
11/10/1400	80.3
12/10/1400	79
13/10/1400	83
14/10/1400	78.4
15/10/1400	79
18/10/1400	78.5
19/10/1400	88.5

تاریخ	مقدار
18/09/1400	80.5
20/09/1400	86.6
21/09/1400	85.9
22/09/1400	86
23/09/1400	86.5
24/09/1400	86.1
25/09/1400	86
27/09/1400	84
28/09/1400	88.5
29/09/1400	84.7
30/09/1400	84.5
01/10/1400	82.6
02/10/1400	89

Mean: 83.651	SD: 3.552	CV%: 4.246
--------------	-----------	------------

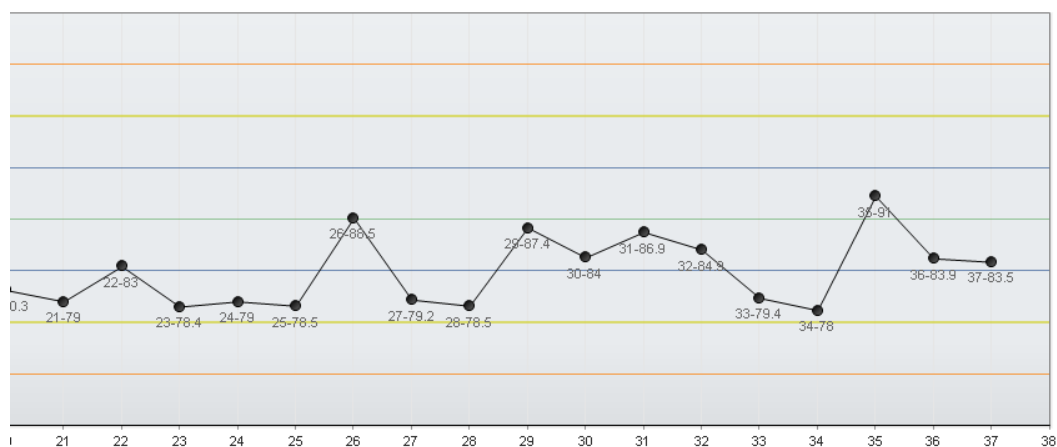

CV% 4.3 SD 5.867 -3SD 70.799 -2SD 76.666 -1SD 82.533 Mean 88.4 1SD 94.267 2SD 100.134 3SD 106.001

جاب

abbott-III

عنوان کنترل

اطلاعات

سری ساخت : 34312203

آرشیو

شروع کنترل : 1400/09/18

مقدار	تاریخ
83.3	1400/10/05
80	1400/10/06
88.5	1400/10/07
83.9	1400/10/08
81.7	1400/10/09
80.3	1400/10/11
79	1400/10/12
83	1400/10/13
78.4	1400/10/14
79	1400/10/15
78.5	1400/10/18
88.5	1400/10/19
79.2	1400/10/20
78.5	1400/10/21
87.4	1400/10/22
84	1400/10/23
86.9	1400/10/25
84.9	1400/10/26
79.4	1400/10/27
78	1400/10/28
91	1400/10/29
83.9	1400/10/30
83.5	1400/11/02

Mean: 83.651 SD: 3.552 CV%: 4.246 6σ

abbott

