

عنوان آزمایش : CA-125

عنوان دستگاه : abbot 34312201 : سری ساخت

عنوان کنترل :

abbot-I

شروع کنترل : 1400/09/18


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
16.601	15.324	14.047	12.77	11.493	10.216	8.939	1.277	4.3

تاریخ	مقدار
30/09/1400	12.1
01/10/1400	11.4
02/10/1400	11.6
04/10/1400	11.2

تاریخ	مقدار
24/09/1400	11.9
25/09/1400	12.2
27/09/1400	12.8
28/09/1400	11.5
29/09/1400	11.9

تاریخ	مقدار
18/09/1400	11.1
20/09/1400	12
21/09/1400	11.6
22/09/1400	11.8
23/09/1400	12.2

Mean: 11.807	SD: 0.451	CV%: 3.823
--------------	-----------	------------

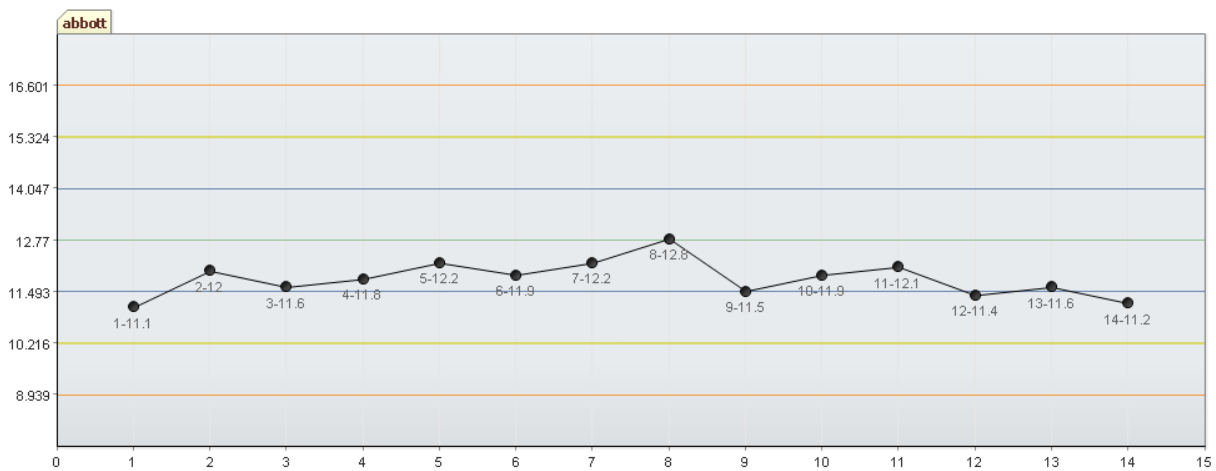

عنوان آزمایش : CA-125

عنوان دستگاه : abbot 34312203 : سری ساخت

عنوان کنترل :

abbot-III

شروع کنترل : 1400/09/18

3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
106.001	100.134	94.267	88.4	82.533	76.666	70.799	5.867	4.3

تاریخ	مقدار
30/09/1400	84.5
01/10/1400	82.6
02/10/1400	82
04/10/1400	83.4

تاریخ	مقدار
24/09/1400	86.1
25/09/1400	86
27/09/1400	84
28/09/1400	88.5
29/09/1400	84.7

تاریخ	مقدار
18/09/1400	80.5
20/09/1400	86.6
21/09/1400	85.9
22/09/1400	86
23/09/1400	86.5

Mean: 84.807	SD: 2.139	CV%: 2.522
--------------	-----------	------------

