

عنوان آزمایش : CA 19-9

عنوان دستگاه : ABBBOTT سری ساخت : 34312201

عنوان کنترل :

شروع کنترل : 1400/09/18

multichem I


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
47.001	43.384	39.767	36.15	32.533	28.916	25.299	3.617	8.5

تاریخ	مقدار
20/10/1400	36.9
21/10/1400	36.5
22/10/1400	35
23/10/1400	36.7
25/10/1400	38.4
26/10/1400	36.9
27/10/1400	38.4
28/10/1400	37
29/10/1400	37.08
30/10/1400	38.9
02/11/1400	36.9
03/11/1400	36
04/11/1400	37.1

تاریخ	مقدار
04/10/1400	39.7
05/10/1400	36
06/10/1400	39.2
07/10/1400	41.3
08/10/1400	39
09/10/1400	41.1
11/10/1400	37.6
12/10/1400	37
13/10/1400	40.1
14/10/1400	34.4
15/10/1400	32.3
18/10/1400	35
19/10/1400	37.1

تاریخ	مقدار
18/09/1400	35.7
20/09/1400	37.2
21/09/1400	36.8
22/09/1400	37.01
23/09/1400	37.5
24/09/1400	39.6
25/09/1400	37
27/09/1400	36.8
28/09/1400	35
29/09/1400	35.9
30/09/1400	36.07
01/10/1400	38.4
02/10/1400	37.4

Mean: 37.23	SD: 1.8	CV%: 4.835
-------------	---------	------------





multichem I عنوان کنترل

CV% 8.5 SD 3.617 -3SD 25.299 -2SD 28.916 -1SD 32.533 Mean 36.15 1SD 39.767 2SD 43.384 3SD 47.001


اطلاعات سری ساخت : 34312201

آرشیو شروع کنترل : 1400/09/18

مقدار	تاریخ
41.3	1400/10/07
39	1400/10/08
41.1	1400/10/09
37.6	1400/10/11
37	1400/10/12
40.1	1400/10/13
34.4	1400/10/14
32.3	1400/10/15
35	1400/10/18
37.1	1400/10/19
36.9	1400/10/20
36.5	1400/10/21
35	1400/10/22
36.7	1400/10/23
38.4	1400/10/25
36.9	1400/10/26
38.4	1400/10/27
37	1400/10/28
37.08	1400/10/29
38.9	1400/10/30
36.9	1400/11/02
36	1400/11/03
37.1	1400/11/04

Mean: 37.23 SD: 1.8 CV%: 4.835 6σ

ABBOTT

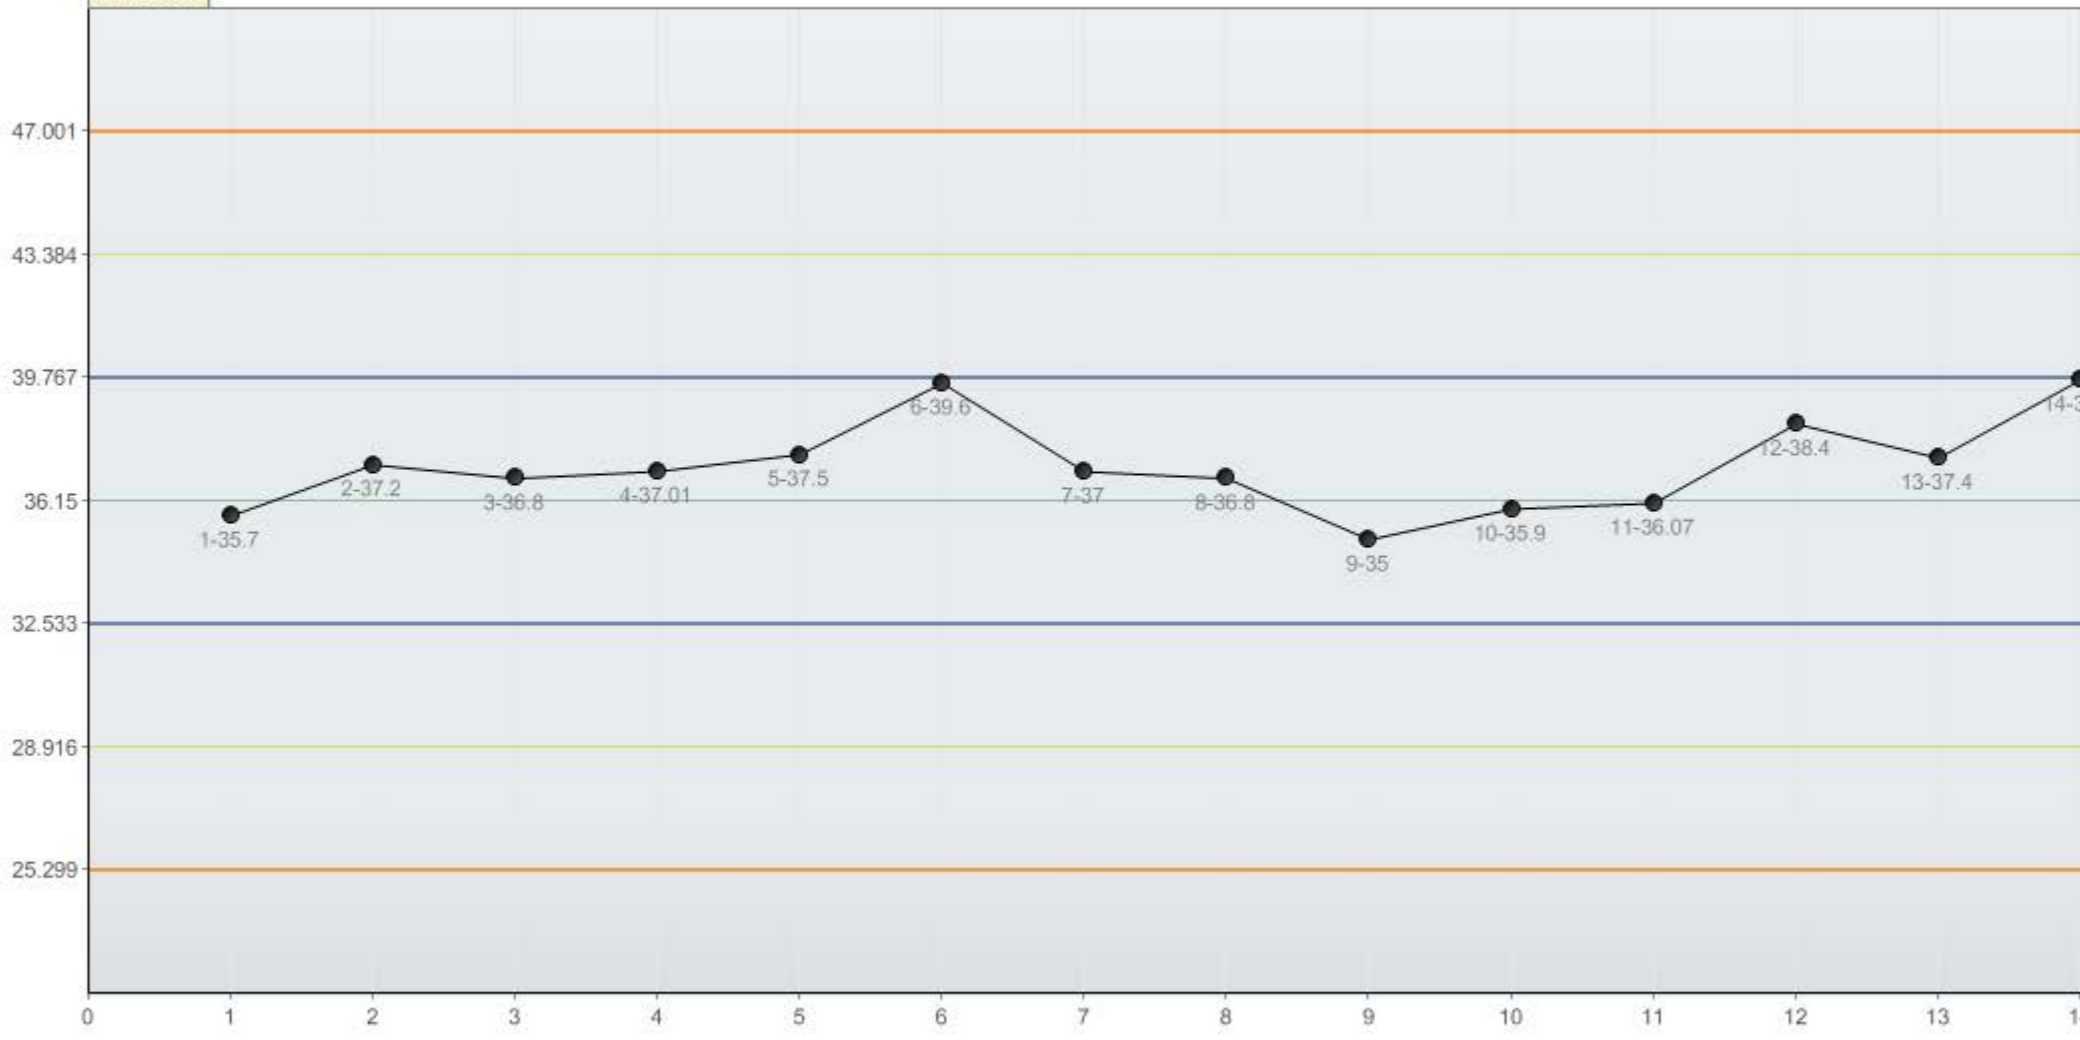

عنوان آزمایش : CA 19-9

عنوان دستگاه : ABBOTT سری ساخت : 34312203

عنوان کنترل :

Multichem II

شروع کنترل : 1400/09/18

3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
144.001	136.034	128.067	120.1	112.133	104.166	96.199	7.967	8.4

تاریخ	مقدار
20/10/1400	123.2
21/10/1400	116.4
22/10/1400	113.7
23/10/1400	120.4
25/10/1400	124.6
26/10/1400	118.3
27/10/1400	119.6
28/10/1400	118
29/10/1400	118.6
30/10/1400	122
02/11/1400	126
03/11/1400	119
04/11/1400	120

تاریخ	مقدار
04/10/1400	135
05/10/1400	131
06/10/1400	135
07/10/1400	127
08/10/1400	136
09/10/1400	124
11/10/1400	121
12/10/1400	120
13/10/1400	125
14/10/1400	110
15/10/1400	110.6
18/10/1400	120.7
19/10/1400	121.7

تاریخ	مقدار
18/09/1400	118.5
20/09/1400	123
21/09/1400	111.9
22/09/1400	124.5
23/09/1400	128.2
24/09/1400	128.3
25/09/1400	114.3
27/09/1400	126.5
28/09/1400	124
29/09/1400	123
30/09/1400	125.8
01/10/1400	119.3
02/10/1400	123.5

Mean: 122.246	SD: 6.127	CV%: 5.012
---------------	-----------	------------



Multichem II

عنوان کنترل

اطلاعات

سری ساخت : 34312203

آرشیو

شروع کنترل : 1400/09/18

مقدار

تاریخ

مقدار	تاریخ
118.5	1400/09/18
123	1400/09/20
111.9	1400/09/21
124.5	1400/09/22
128.2	1400/09/23
128.3	1400/09/24
114.3	1400/09/25
126.5	1400/09/27
124	1400/09/28
123	1400/09/29
125.8	1400/09/30
119.3	1400/10/01
123.5	1400/10/02
135	1400/10/04
131	1400/10/05
135	1400/10/06
127	1400/10/07
136	1400/10/08
124	1400/10/09
121	1400/10/11
120	1400/10/12
125	1400/10/13
110	1400/10/14
110.6	1400/10/15

Mean: 122.246

SD: 6.127

CV%: 5.012

6σ

CV% 8.4

SD 7.967

-3SD 96.199

-2SD 104.166

-1SD 112.133

Mean 120.1

1SD 128.067

2SD 136.034

3SD 144.001

جاب

ABBOTT

