


Multichem-1 عنوان کنترل

اطلاعات سری ساخت : 34312201
 آرشیو شروع کنترل : 1400/09/18

CV% 3.6 SD 0.2 -3SD 2.39 -2SD 2.59 -1SD 2.79 Mean 2.99 1SD 3.19 2SD 3.39 3SD 3.59

مقدار	تاریخ
2.81	1400/09/18
2.99	1400/09/20
2.91	1400/09/21
3.06	1400/09/22
2.87	1400/09/23
2.84	1400/09/24
2.67	1400/09/25
2.81	1400/09/27
2.97	1400/09/28
2.93	1400/09/29
3.11	1400/09/30
2.93	1400/10/01
2.9	1400/10/02
2.85	1400/10/04
3.02	1400/10/05
3.11	1400/10/06
3.07	1400/10/07
3.02	1400/10/08
2.91	1400/10/09
3.32	1400/10/11
3.2	1400/10/12
3.26	1400/10/13
2.96	1400/10/14
2.6	1400/10/15
2.84	1400/10/18

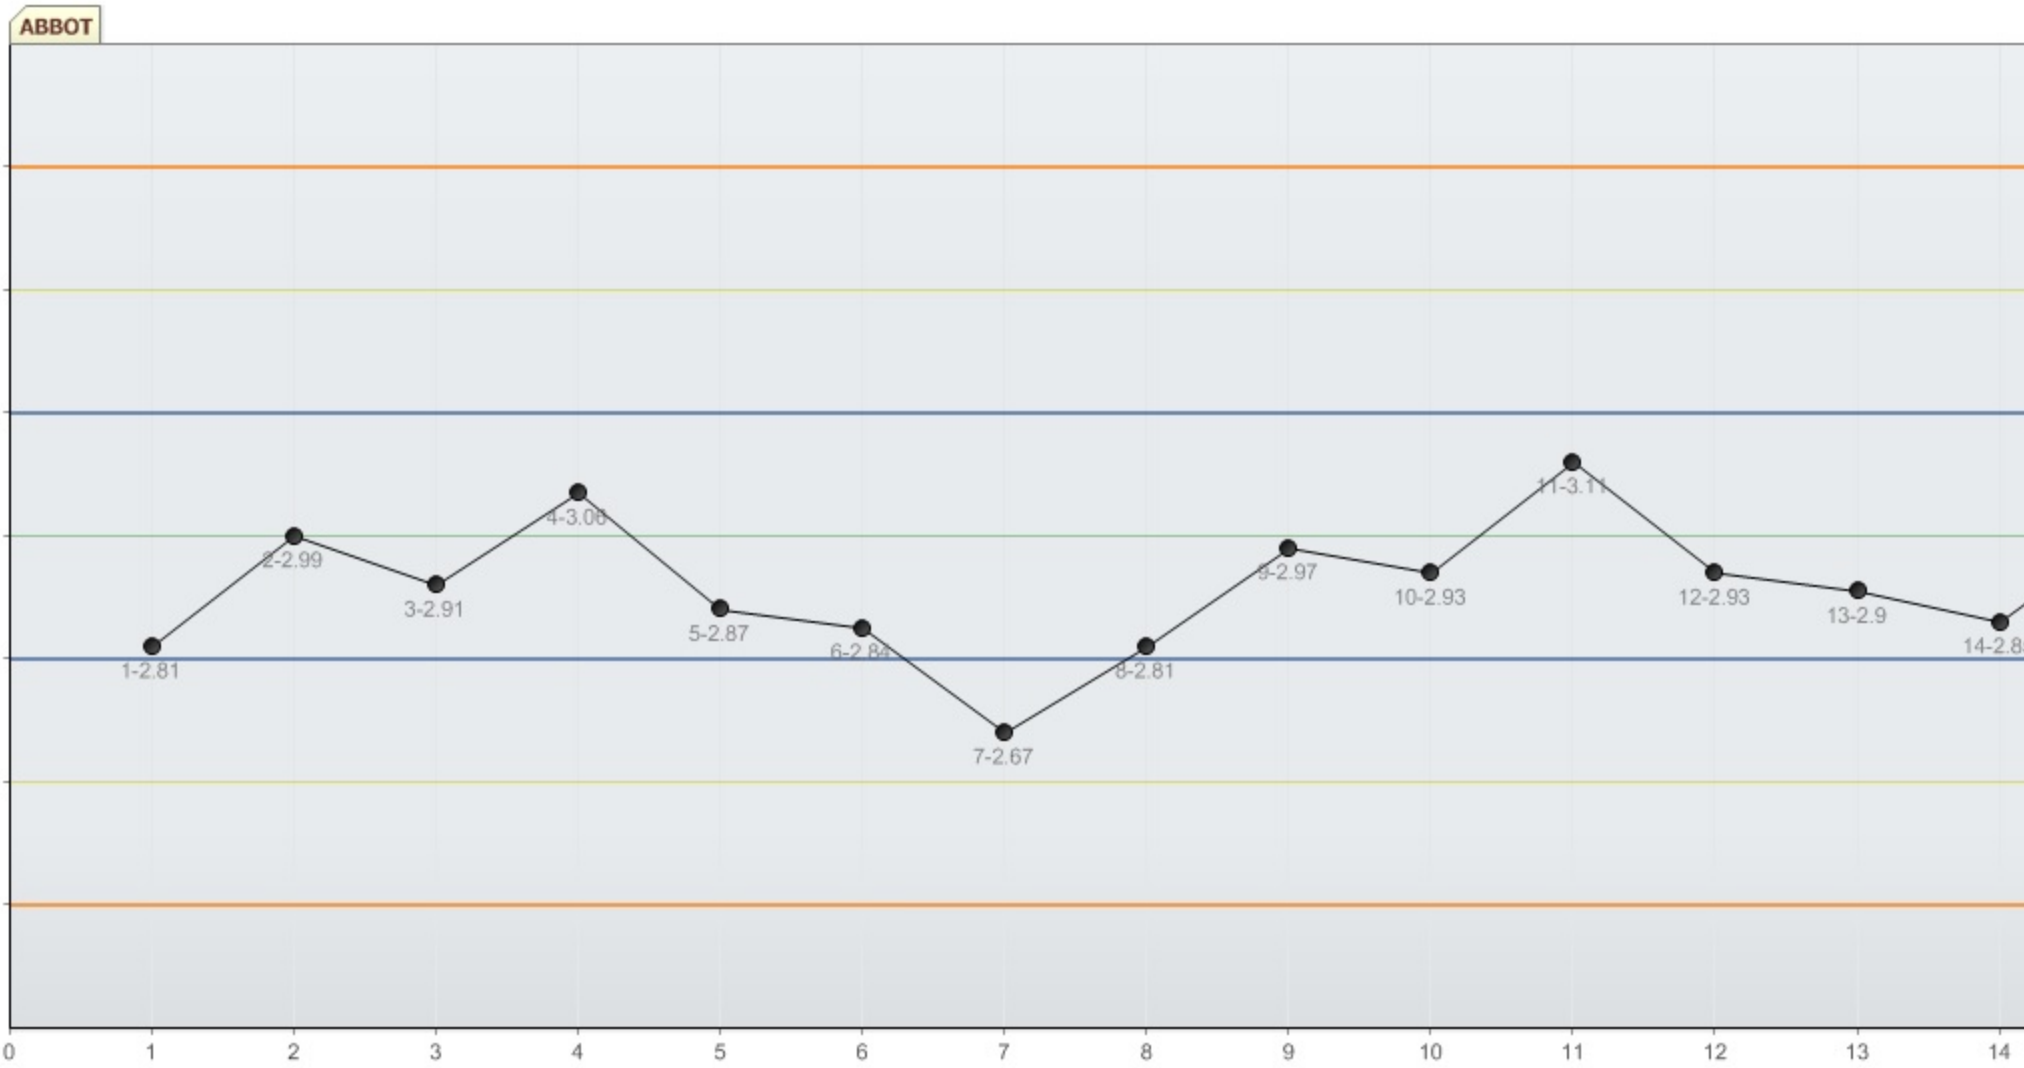

Mean: 2.941 SD: 0.147 CV%: 4.994 **6σ**

عنوان آزمایش : CEA
عنوان دستگاه : ABBOT سری ساخت : 34312201

عنوان کنترل : Multichem-1
شروع کنترل : 1400/09/18


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
3.59	3.39	3.19	2.99	2.79	2.59	2.39	0.2	3.6

تاریخ	مقدار
20/10/1400	2.92
21/10/1400	2.98
22/10/1400	3.03
23/10/1400	2.82
25/10/1400	2.88
26/10/1400	2.84
27/10/1400	2.9
28/10/1400	2.89
29/10/1400	3.01
30/10/1400	2.79

تاریخ	مقدار
04/10/1400	2.85
05/10/1400	3.02
06/10/1400	3.11
07/10/1400	3.07
08/10/1400	3.02
09/10/1400	2.91
11/10/1400	3.32
12/10/1400	3.2
13/10/1400	3.26
14/10/1400	2.96
15/10/1400	2.6
18/10/1400	2.84
19/10/1400	2.86

تاریخ	مقدار
18/09/1400	2.81
20/09/1400	2.99
21/09/1400	2.91
22/09/1400	3.06
23/09/1400	2.87
24/09/1400	2.84
25/09/1400	2.67
27/09/1400	2.81
28/09/1400	2.97
29/09/1400	2.93
30/09/1400	3.11
01/10/1400	2.93
02/10/1400	2.9

Mean: 2.941	SD: 0.147	CV%: 4.994
-------------	-----------	------------

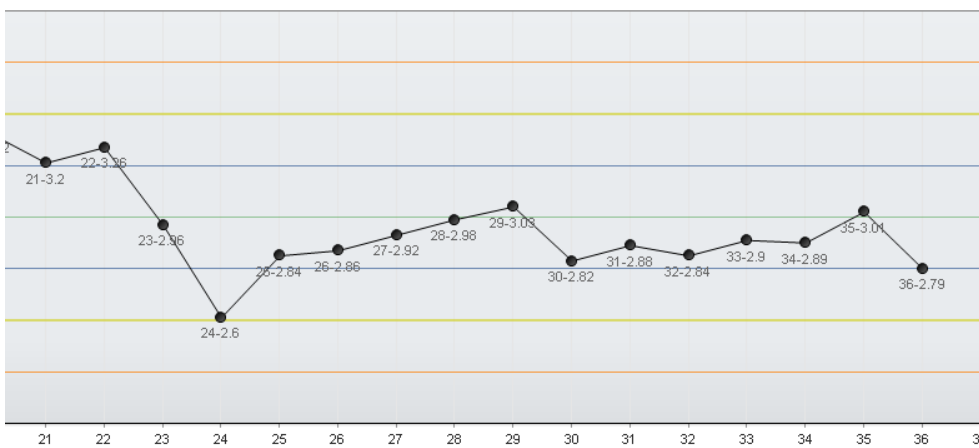

Multichem-3

عنوان کنترل

CV% 3.6 SD 3.317 -3SD 39.899 -2SD 43.216 -1SD 46.533 Mean 49.85 1SD 53.167 2SD 56.484 3SD 59.801

چاپ

اطلاعات

سری ساخت : 34312203

آرشیو

شروع کنترل : 1400/09/18

مقدار تاریخ

مقدار	تاریخ
50.6	1400/09/18
48.5	1400/09/20
46.7	1400/09/21
48.9	1400/09/22
50.2	1400/09/23
50.1	1400/09/24
48.7	1400/09/25
49.5	1400/09/27
50.7	1400/09/28
50.8	1400/09/29
46.3	1400/09/30
48.5	1400/10/01
48.7	1400/10/02
48.9	1400/10/04
50.5	1400/10/05
50.8	1400/10/06
47.9	1400/10/07
49.3	1400/10/08
49.2	1400/10/09
50.2	1400/10/11
48.8	1400/10/12
48.7	1400/10/13
45.6	1400/10/14
48.3	1400/10/15


Mean: 49.1

SD: 1.379

CV%: 2.808

6σ

ABBOTT

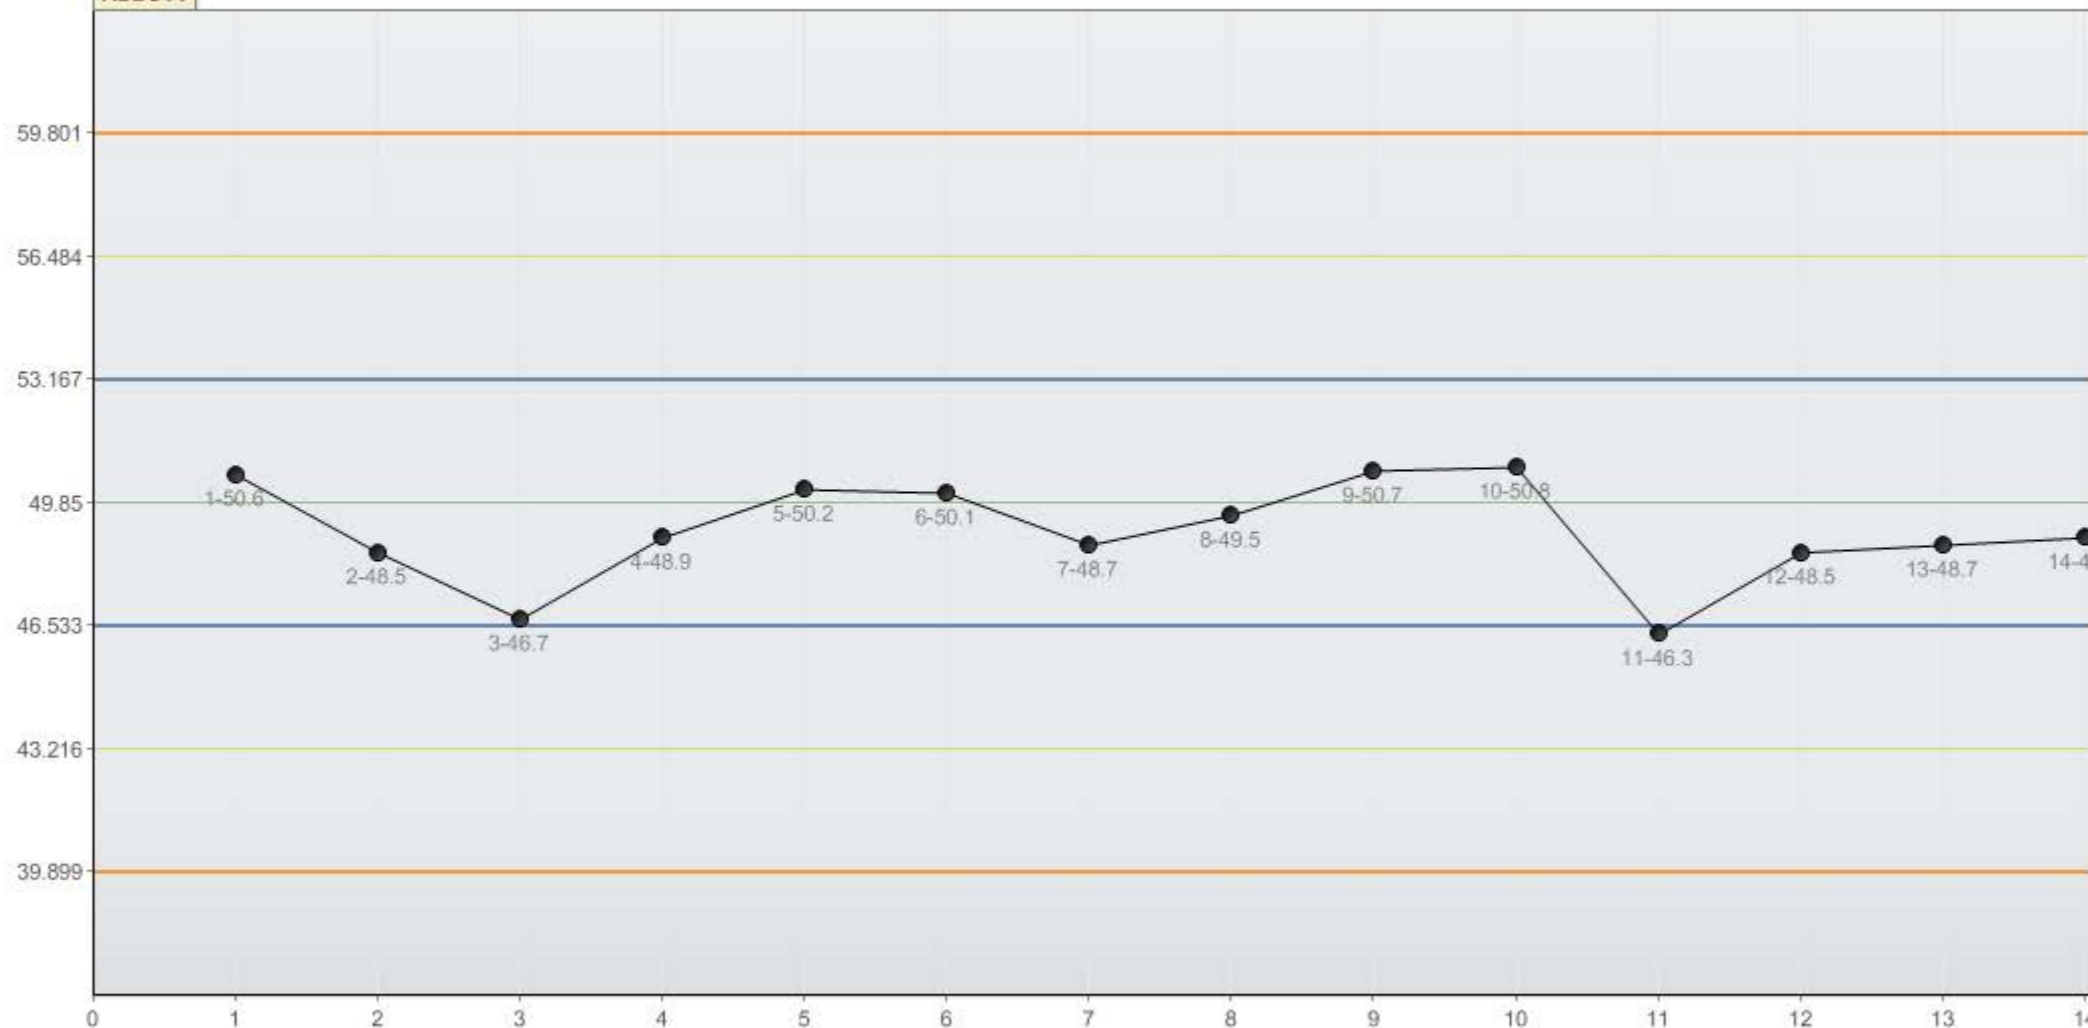

عنوان آزمایش : CEA

عنوان دستگاه : ABBOTT

سری ساخت : 34312203

عنوان کنترل :

شروع کنترل : 1400/09/18

Multichem-3

3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
59.801	56.484	53.167	49.85	46.533	43.216	39.899	3.317	3.6

تاریخ	مقدار
20/10/1400	49.9
21/10/1400	50.8
22/10/1400	49.3
23/10/1400	49
25/10/1400	47.5
26/10/1400	49.4
27/10/1400	49.8
28/10/1400	51.1
29/10/1400	49.8
30/10/1400	48
02/11/1400	47.3
03/11/1400	49.3
04/11/1400	51.8

تاریخ	مقدار
04/10/1400	48.9
05/10/1400	50.5
06/10/1400	50.8
07/10/1400	47.9
08/10/1400	49.3
09/10/1400	49.2
11/10/1400	50.2
12/10/1400	48.8
13/10/1400	48.7
14/10/1400	45.6
15/10/1400	48.3
18/10/1400	48
19/10/1400	47.5

تاریخ	مقدار
18/09/1400	50.6
20/09/1400	48.5
21/09/1400	46.7
22/09/1400	48.9
23/09/1400	50.2
24/09/1400	50.1
25/09/1400	48.7
27/09/1400	49.5
28/09/1400	50.7
29/09/1400	50.8
30/09/1400	46.3
01/10/1400	48.5
02/10/1400	48.7

Mean: 49.1	SD: 1.379	CV%: 2.808
------------	-----------	------------

