

عنوان آزمایش : CMV Ab (IgG)-CLIA
عنوان دستگاه : abbot

01727 : سری ساخت FN00

عنوان کنترل : abbot-1
شروع کنترل : 1399/05/22


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
35.259	34.225	33.191	32.157	31.123	30.089	29.055	1.034	3.215

تاریخ	مقدار
22/04/1400	30.9
23/04/1400	32.3
24/04/1400	31
26/04/1400	30.6
27/04/1400	31
28/04/1400	32

تاریخ	مقدار
12/04/1400	32
13/04/1400	33
14/04/1400	31.9
15/04/1400	30.5
16/04/1400	31
17/04/1400	30.3
19/04/1400	32
20/04/1400	31
21/04/1400	30.8

تاریخ	مقدار
01/04/1400	32.9
02/04/1400	32
03/04/1400	31
05/04/1400	30.9
06/04/1400	31
07/04/1400	32
08/04/1400	31
09/04/1400	30.4
10/04/1400	32.3

Mean: 31.408	SD: 0.783	CV%: 2.494
--------------	-----------	------------

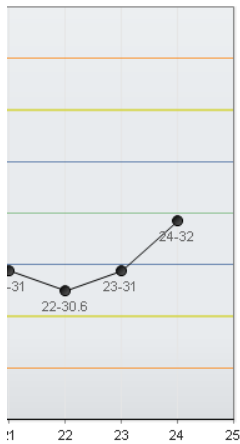



V% 3.215 SD 1.034 -3SD 29.055 -2SD 30.089 -1SD 31.123 Mean 32.157 1SD 33.191 2SD 34.225 3SD 35.259 چاپ

abbott

