

عنوان آزمایش : FSH

عنوان دستگاه : abbott سری ساخت : 33402201

عنوان کنترل : abbott-1

شروع کنترل : 1400/02/01


| 3SD | 2SD | 1SD | MEAN | -1SD | -2SD | -3SD | SD | CV% |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|
| 7.284 | 6.959 | 6.634 | 6.309 | 5.984 | 5.659 | 5.334 | 0.325 | 5.157 |

| تاریخ | مقدار |
|------------|-------|
| 22/04/1400 | 6.1 |
| 23/04/1400 | 6.2 |
| 24/04/1400 | 6.13 |
| 26/04/1400 | 5.96 |
| 27/04/1400 | 6.35 |
| 28/04/1400 | 5.87 |

| تاریخ | مقدار |
|------------|-------|
| 12/04/1400 | 5.75 |
| 13/04/1400 | 5.9 |
| 14/04/1400 | 6.32 |
| 15/04/1400 | 5.95 |
| 16/04/1400 | 5.8 |
| 17/04/1400 | 5.75 |
| 19/04/1400 | 6 |
| 20/04/1400 | 6.34 |
| 21/04/1400 | 5.9 |

| تاریخ | مقدار |
|------------|-------|
| 01/04/1400 | 6.3 |
| 02/04/1400 | 6.03 |
| 03/04/1400 | 5.93 |
| 05/04/1400 | 6.4 |
| 06/04/1400 | 5.82 |
| 07/04/1400 | 6.07 |
| 08/04/1400 | 6 |
| 09/04/1400 | 5.9 |
| 10/04/1400 | 5.99 |

| | | |
|-------------|-----------|------------|
| Mean: 6.032 | SD: 0.197 | CV%: 3.266 |
|-------------|-----------|------------|

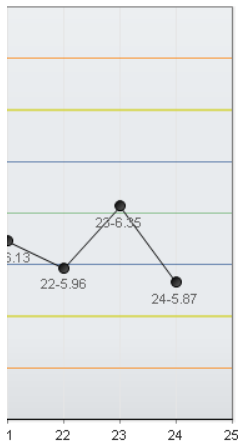



V% 5.157 SD 0.325 -3SD 5.334 -2SD 5.659 -1SD 5.984 Mean 6.309 1SD 6.634 2SD 6.959 3SD 7.284

چاپ

abbott

