

عنوان آزمایش : Free PSA -CLIA
عنوان دستگاه : abbot

سری ساخت : 34312201

عنوان کنترل : abbot-I
شروع کنترل: 1400/09/18

3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
0.274	0.253	0.232	0.211	0.19	0.169	0.148	0.021	4.7

تاریخ	مقدار
20/10/1400	0.217
21/10/1400	0.178
22/10/1400	0.185
23/10/1400	0.186
25/10/1400	0.194
26/10/1400	0.18
27/10/1400	0.215
29/10/1400	0.185
30/10/1400	0.177
02/11/1400	0.181
03/11/1400	0.192
04/11/1400	0.183

تاریخ	مقدار
04/10/1400	0.186
05/10/1400	0.211
06/10/1400	0.187
07/10/1400	0.186
08/10/1400	0.212
09/10/1400	0.196
11/10/1400	0.188
12/10/1400	0.189
13/10/1400	0.1996
14/10/1400	0.186
15/10/1400	0.178
18/10/1400	0.179
19/10/1400	0.191

تاریخ	مقدار
18/09/1400	0.196
20/09/1400	0.187
21/09/1400	0.201
22/09/1400	0.186
23/09/1400	0.2
24/09/1400	0.186
25/09/1400	0.218
27/09/1400	0.186
28/09/1400	0.195
29/09/1400	0.188
30/09/1400	0.201
01/10/1400	0.178
02/10/1400	0.181

Mean: 0.191	SD: 0.011	CV%: 5.948
-------------	-----------	------------




CV% 4.7 SD 0.021 -3SD 0.148 -2SD 0.169 -1SD 0.19 Mean 0.211 1SD 0.232 2SD 0.253 3SD 0.274

abbott-I عنوان کنترل

اطلاعات سری ساخت : 34312201
آرشیو شروع کنترل : 1400/09/18

مقدار	تاریخ
0.196	1400/09/18
0.187	1400/09/20
0.201	1400/09/21
0.186	1400/09/22
0.2	1400/09/23
0.186	1400/09/24
0.218	1400/09/25
0.186	1400/09/27
0.195	1400/09/28
0.188	1400/09/29
0.201	1400/09/30
0.178	1400/10/01
0.181	1400/10/02
0.186	1400/10/04
0.211	1400/10/05
0.187	1400/10/06
0.186	1400/10/07
0.212	1400/10/08
0.196	1400/10/09
0.188	1400/10/11
0.189	1400/10/12
0.1996	1400/10/13
0.186	1400/10/14
0.178	1400/10/15

Mean: 0.191 SD: 0.011 CV%: 5.948 **6σ**

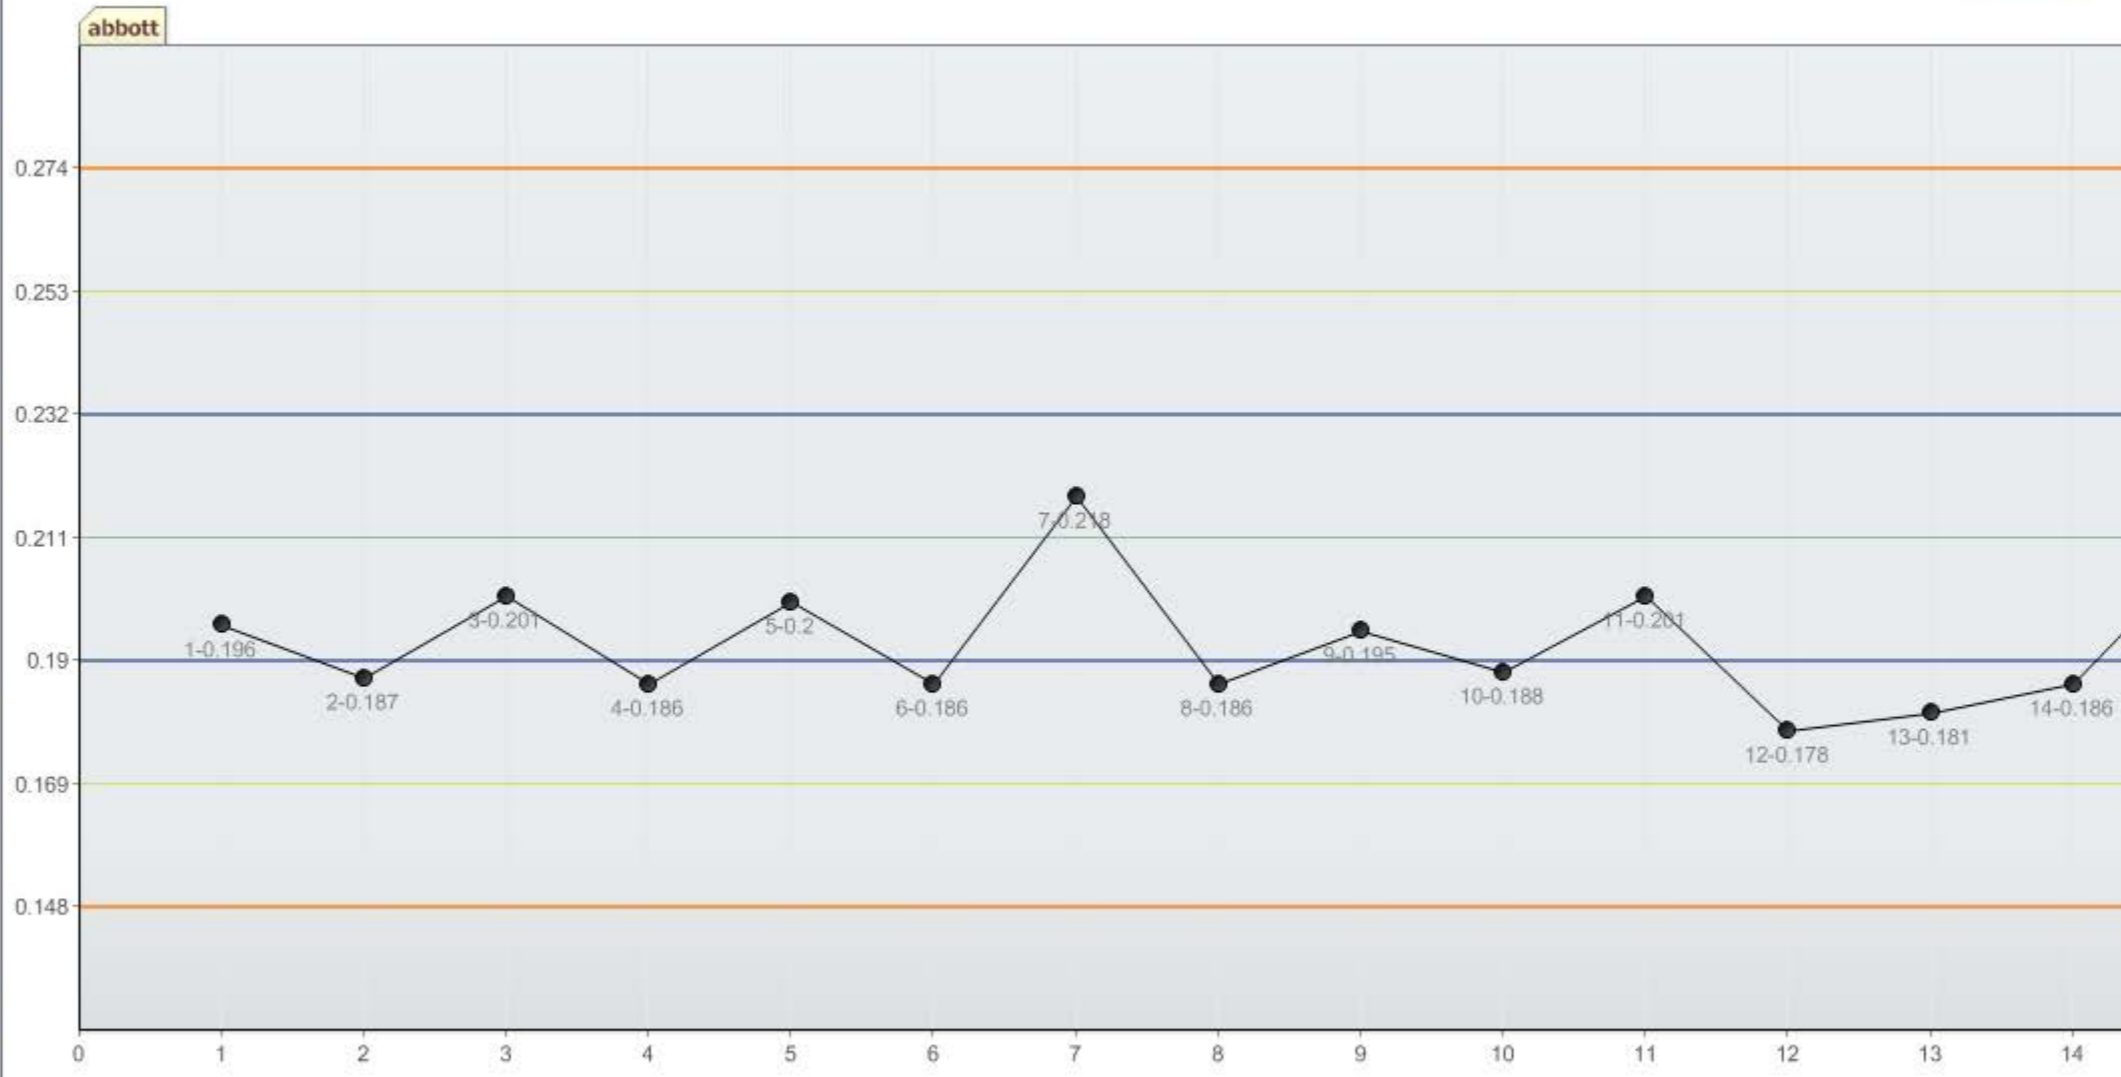

عنوان آزمایش : Free PSA -CLIA
عنوان دستگاه : abbott

سری ساخت : 34312203

عنوان کنترل : abbot-III
شروع کنترل : 1400/09/18

3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
15.099	14.266	13.433	12.6	11.767	10.934	10.101	0.833	4.7

تاریخ	مقدار
20/10/1400	13
21/10/1400	11.9
22/10/1400	12.3
23/10/1400	12.6
25/10/1400	12
26/10/1400	12.3
27/10/1400	12.2
29/10/1400	12.9
30/10/1400	11.8
02/11/1400	12.3
03/11/1400	12.2
04/11/1400	12.3

تاریخ	مقدار
04/10/1400	12.7
05/10/1400	13.2
06/10/1400	12.8
07/10/1400	12.6
08/10/1400	12.8
09/10/1400	12.3
11/10/1400	12.3
12/10/1400	12.7
13/10/1400	12.3
14/10/1400	13.5
15/10/1400	12.3
18/10/1400	11.9
19/10/1400	12.8

تاریخ	مقدار
18/09/1400	12.7
20/09/1400	12.3
21/09/1400	12.1
22/09/1400	12.4
23/09/1400	12.2
24/09/1400	12.8
25/09/1400	12.4
27/09/1400	12.9
28/09/1400	13.1
29/09/1400	12
30/09/1400	12.2
01/10/1400	12.5
02/10/1400	11.9

Mean: 12.461	SD: 0.397	CV%: 3.186
--------------	-----------	------------



abbott-III

عنوان کنترل

CV% 4.7 SD 0.833 -3SD 10.101 -2SD 10.934 -1SD 11.767 Mean 12.6 1SD 13.433 2SD 14.266 3SD 15.099 چاپ

اطلاعات

سری ساخت : 34312203

آرشیو

شروع کنترل : 1400/09/18

مقدار	تاریخ
12.7	1400/09/18
12.3	1400/09/20
12.1	1400/09/21
12.4	1400/09/22
12.2	1400/09/23
12.8	1400/09/24
12.4	1400/09/25
12.9	1400/09/27
13.1	1400/09/28
12	1400/09/29
12.2	1400/09/30
12.5	1400/10/01
11.9	1400/10/02
12.7	1400/10/04
13.2	1400/10/05
12.8	1400/10/06
12.6	1400/10/07
12.8	1400/10/08
12.3	1400/10/09
12.3	1400/10/11
12.7	1400/10/12
12.3	1400/10/13
13.5	1400/10/14
12.3	1400/10/15

Mean: 12.461 SD: 0.397 CV%: 3.186 6σ

