

عنوان آزمایش : Free PSA -CLIA
عنوان دستگاه : abbot

سری ساخت : 33402201

عنوان کنترل : abbot-I
شروع کنترل : 1400/02/01


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
0.411	0.403	0.395	0.387	0.379	0.371	0.363	0.008	2.06

تاریخ	مقدار
22/04/1400	0.4
23/04/1400	0.398
24/04/1400	0.4
26/04/1400	0.395
27/04/1400	0.4
28/04/1400	0.384
31/04/1400	0.375

تاریخ	مقدار
12/04/1400	0.38
13/04/1400	0.394
14/04/1400	0.4
15/04/1400	0.394
16/04/1400	0.399
17/04/1400	0.4
19/04/1400	0.382
20/04/1400	0.4
21/04/1400	0.39

تاریخ	مقدار
01/04/1400	0.385
02/04/1400	0.379
03/04/1400	0.377
05/04/1400	0.373
06/04/1400	0.378
07/04/1400	0.388
08/04/1400	0.375
09/04/1400	0.377
10/04/1400	0.4

Mean: 0.389	SD: 0.01	CV%: 2.595
-------------	----------	------------

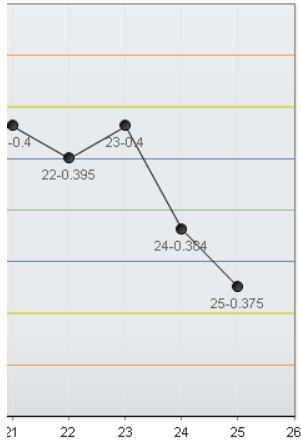



% 2.06 SD 0.008 -3SD 0.363 -2SD 0.371 -1SD 0.379 Mean 0.387 1SD 0.395 2SD 0.403 3SD 0.411

جاب

