

عنوان آزمایش : PSA -CLIA

عنوان دستگاه : abbott

سری ساخت : 34312201

عنوان کنترل :

abbott-1

شروع کنترل : 1400/09/18


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
0.73	0.674	0.618	0.562	0.506	0.45	0.394	0.056	3.6

تاریخ	مقدار
05/10/1400	0.6
06/10/1400	0.524
07/10/1400	0.548
08/10/1400	0.517

تاریخ	مقدار
27/09/1400	0.56
28/09/1400	0.582
29/09/1400	0.517
30/09/1400	0.602
01/10/1400	0.573
02/10/1400	0.548
04/10/1400	0.523

تاریخ	مقدار
18/09/1400	0.571
20/09/1400	0.552
21/09/1400	0.509
22/09/1400	0.557
23/09/1400	0.534
24/09/1400	0.567
25/09/1400	0.562

Mean: 0.553	SD: 0.028	CV%: 5.042
-------------	-----------	------------

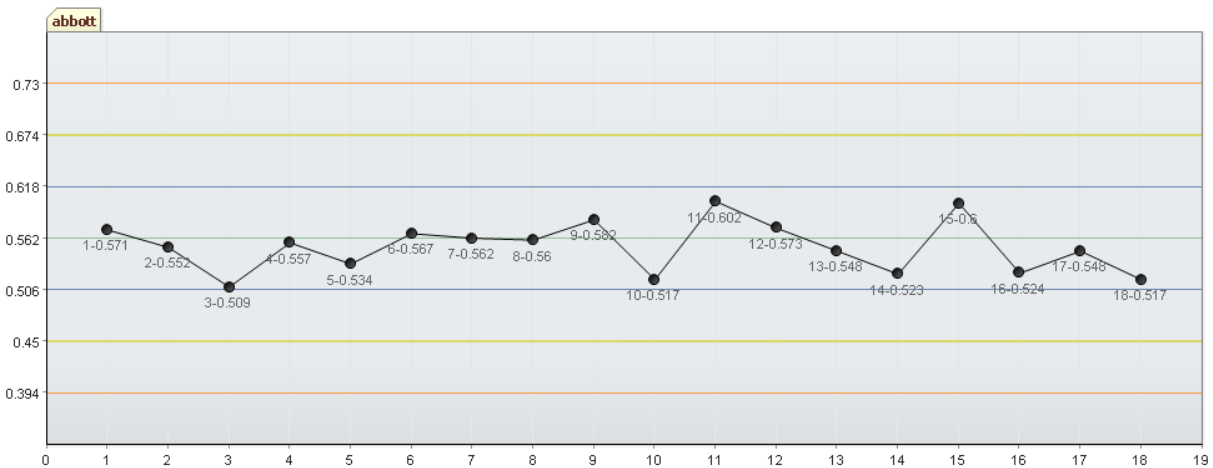

عنوان آزمایش : PSA -CLIA

عنوان دستگاه : Simense

سری ساخت : 40383

عنوان کنترل :

biorad III

شروع کنترل : 1400/10/09

3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
25.3	23	20.7	18.4	16.1	13.8	11.5	2.3	0

تاریخ	مقدار
27/10/1400	17.3
28/10/1400	16.9
29/10/1400	17.3

تاریخ	مقدار
19/10/1400	18.5
20/10/1400	16.5
22/10/1400	17.3
23/10/1400	17.4
25/10/1400	17.4
26/10/1400	18

تاریخ	مقدار
11/10/1400	18.7
12/10/1400	16.3
13/10/1400	17.1
14/10/1400	17
15/10/1400	16.9
18/10/1400	17

Mean: 17.329	SD: 0.679	CV%: 3.917
--------------	-----------	------------

