

عنوان آزمایش : PSA -CLIA

عنوان دستگاه : abbot

سری ساخت : 33402201

عنوان کنترل :

abbott-1

شروع کنترل : 1400/02/01


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
0.775	0.749	0.723	0.697	0.671	0.645	0.619	0.026	3.8

تاریخ	مقدار
22/04/1400	0.72
23/04/1400	0.74
24/04/1400	0.739
26/04/1400	0.684
27/04/1400	0.663
28/04/1400	0.683
31/04/1400	0.739

تاریخ	مقدار
12/04/1400	0.678
13/04/1400	0.67
14/04/1400	0.676
15/04/1400	0.665
16/04/1400	0.692
17/04/1400	0.682
19/04/1400	0.676
20/04/1400	0.704
21/04/1400	0.691


تاریخ	مقدار
01/04/1400	0.655
02/04/1400	0.66
03/04/1400	0.684
05/04/1400	0.741
06/04/1400	0.672
07/04/1400	0.735
08/04/1400	0.746
09/04/1400	0.714
10/04/1400	0.66

Mean: 0.695	SD: 0.03	CV%: 4.358
-------------	----------	------------

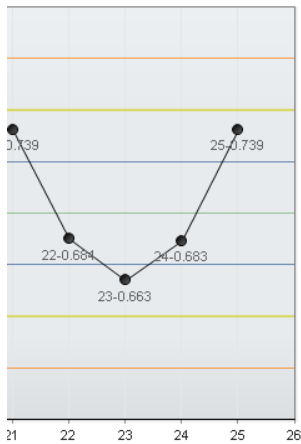



% 3.8 SD 0.026 -3SD 0.619 -2SD 0.645 -1SD 0.671 Mean 0.697 1SD 0.723 2SD 0.749 3SD 0.775



abbott

