

عنوان آزمایش : PSA -CLIA

عنوان دستگاه : abbot

سری ساخت : 34312201

عنوان کنترل :

abbot-1

شروع کنترل : 1400/09/18


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
0.73	0.674	0.618	0.562	0.506	0.45	0.394	0.056	3.6

تاریخ	مقدار
30/09/1400	0.602
01/10/1400	0.573
02/10/1400	0.548
04/10/1400	0.523

تاریخ	مقدار
24/09/1400	0.567
25/09/1400	0.562
27/09/1400	0.56
28/09/1400	0.582
29/09/1400	0.517

تاریخ	مقدار
18/09/1400	0.571
20/09/1400	0.552
21/09/1400	0.509
22/09/1400	0.557
23/09/1400	0.534

Mean: 0.554	SD: 0.026	CV%: 4.699
-------------	-----------	------------

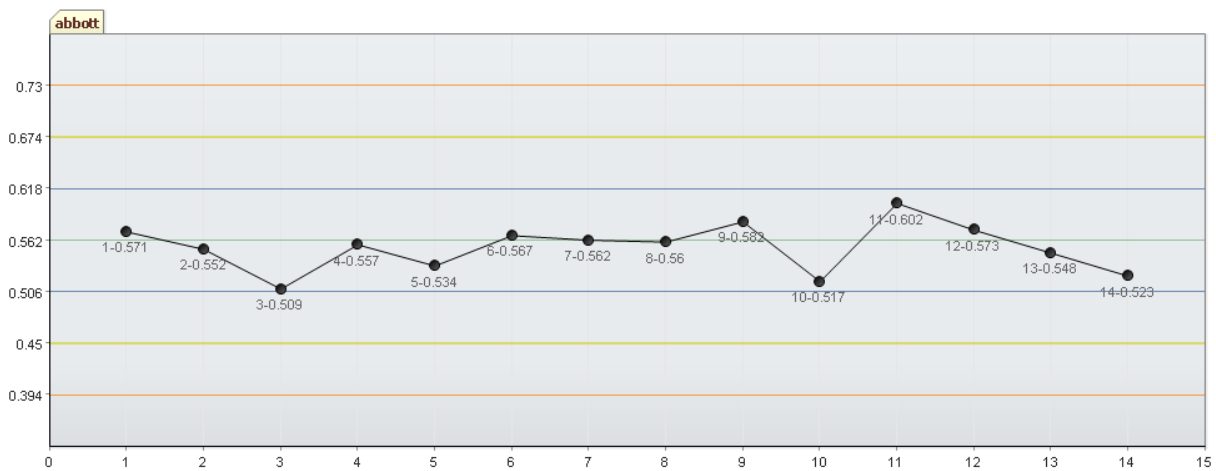

عنوان آزمایش : PSA -CLIA

عنوان دستگاه : abbot

سری ساخت : 34312201

عنوان کنترل :

abbot-3

شروع کنترل : 1400/09/18

3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
30.299	28.616	26.933	25.25	23.567	21.884	20.201	1.683	3.6

تاریخ	مقدار
30/09/1400	27
01/10/1400	24.3
02/10/1400	26.5
04/10/1400	25.2

تاریخ	مقدار
24/09/1400	26.2
25/09/1400	25.4
27/09/1400	26.8
28/09/1400	25.7
29/09/1400	24.7

تاریخ	مقدار
18/09/1400	26.5
20/09/1400	26.6
21/09/1400	26.5
22/09/1400	26.9
23/09/1400	27.3

Mean: 26.114	SD: 0.911	CV%: 3.487
--------------	-----------	------------

