

عنوان آزمایش : Toxoplasma Ab (IgM)-
CLIA

عنوان کنترل : ABBOTT-3

عنوان دستگاه : ABBOTT

BR00 سری ساخت : 13015

شروع کنترل: 1399/06/19


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
2.014	1.924	1.834	1.744	1.654	1.564	1.474	0.09	5.167

تاریخ	مقدار
22/04/1400	1.87
23/04/1400	1.75
24/04/1400	1.8
26/04/1400	1.86
27/04/1400	1.75
28/04/1400	1.8

تاریخ	مقدار
12/04/1400	1.86
13/04/1400	1.64
14/04/1400	1.79
15/04/1400	1.85
16/04/1400	1.87
17/04/1400	1.68
19/04/1400	1.8
20/04/1400	1.69
21/04/1400	1.84

تاریخ	مقدار
01/04/1400	1.63
02/04/1400	1.6
03/04/1400	1.72
05/04/1400	1.75
06/04/1400	1.67
07/04/1400	1.78
08/04/1400	1.8
09/04/1400	1.65
10/04/1400	1.84

Mean: 1.762	SD: 0.084	CV%: 4.777
-------------	-----------	------------

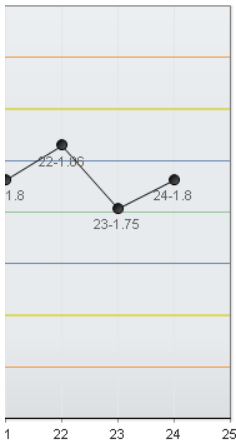



% 5.167 SD 0.09 -3SD 1.474 -2SD 1.564 -1SD 1.654 Mean 1.744 1SD 1.834 2SD 1.924 3SD 2.014 چاپ

ABBOTT

